

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
 Data File : BG024268.D
 Acq On : 11 Oct 2016 15:42
 Operator : UM/SJ
 Sample : H5113-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDP78

Quant Time: Oct 12 04:33:30 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 04:32:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	155670	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	649044	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	500279	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.74	188	1502721	20.00	ng/ul	0.09
75) Chrysene-d12	21.94	240	1294726	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1314242	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	5111	1.56	ng/uL	0.00
5) Phenol-d5	7.42	99	104147	7.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	260120	26.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	234683	23.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	175239	14.92	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	145833	31.66	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	167183	32.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	288758	25.73	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	10737	0.91	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1052214	30.12	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1214138	30.34	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	44991	7.26	ng/ul	0.00
57) Fluorene-d10	15.89	176	987422	29.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	202372	22.41	ng/ul	0.00
70) Anthracene-d10	17.74	188	1502158	22.13	ng/ul	0.00
76) Pyrene-d10	20.01	212	1803718	29.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	1824365	30.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.35	163	49256	1.44	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
Data File : BG024268.D
Acq On : 11 Oct 2016 15:42
Operator : UM/SJ
Sample : H5113-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDP78

Quant Time: Oct 12 04:33:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 04:32:24 2016
Response via : Initial Calibration

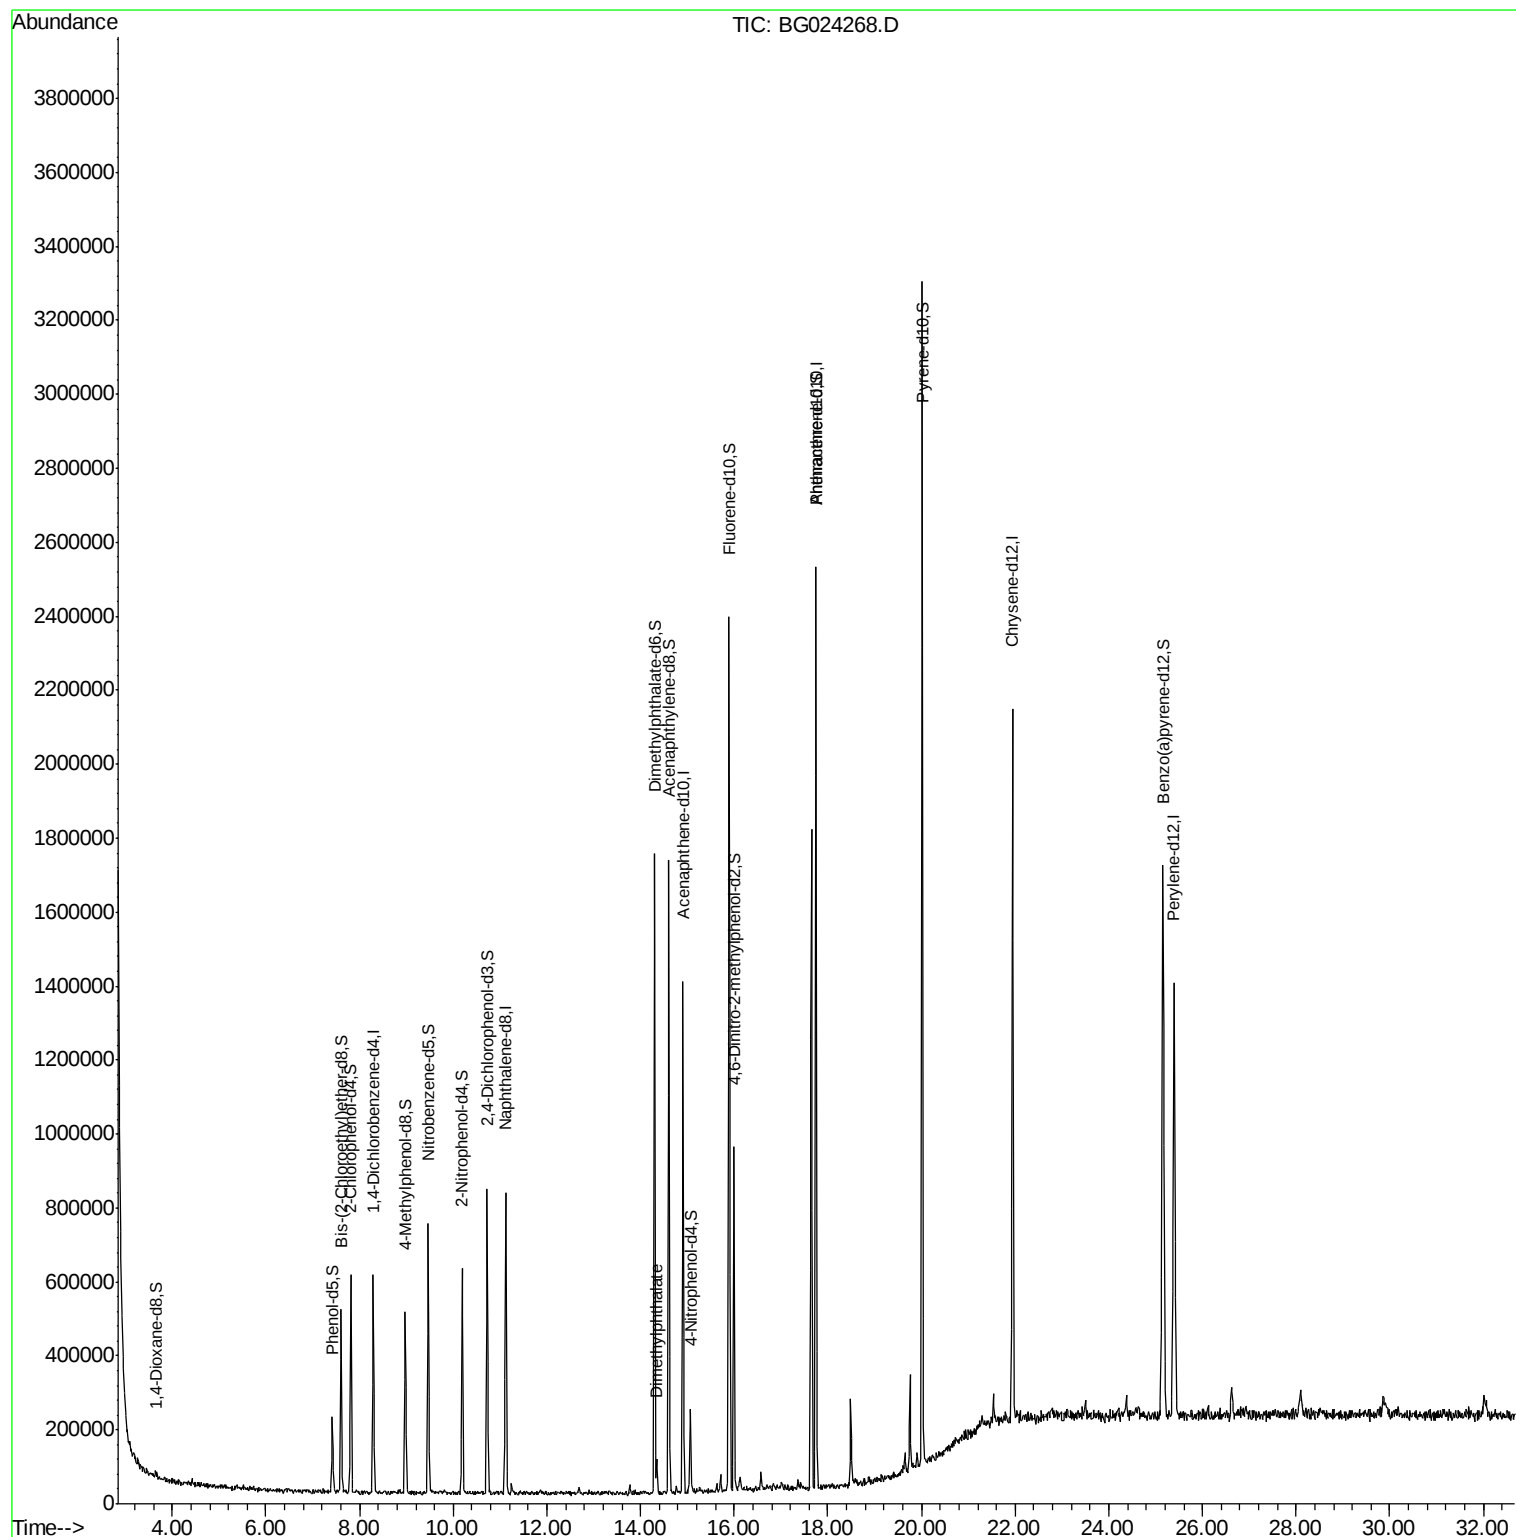

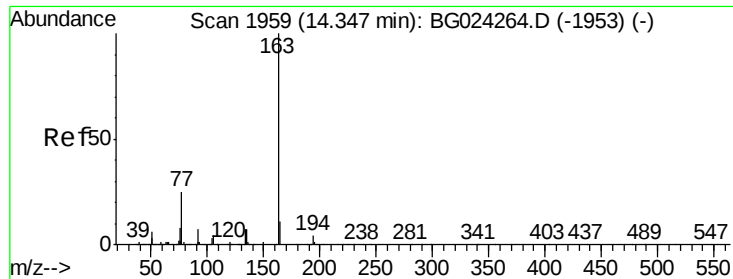

#44

Dimethylphthalate

Concen: 1.44 ng/ul

RT: 14.35 min Scan# 1959

Delta R.T. 0.00 min

Lab File: BG024268.D

Acq: 11 Oct 2016 15:42

Instrument :

BNA_G

ClientSampleId :

BDP78


Tgt Ion:163 Resp: 49256

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 15.0 9.0 13.4#

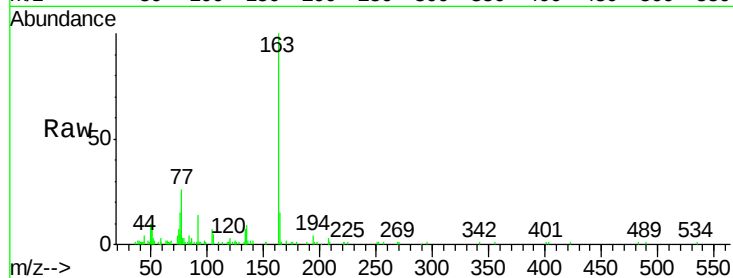

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

