

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
 Data File : BG024271.D
 Acq On : 11 Oct 2016 18:57
 Operator : UM/SJ
 Sample : H5113-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDP72

Quant Time: Oct 12 04:50:42 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 04:50:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	142255	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	602575	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	476886	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1085735	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1248699	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1272605	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	5016	1.67	ng/uL	0.00
5) Phenol-d5	7.41	99	102106	7.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	261077	29.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	225848	24.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	173165	16.14	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	140054	32.75	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	159554	33.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	289714	27.80	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	3250	0.30	ng/ul	0.02
43) Dimethylphthalate-d6	14.30	166	1074375	32.27	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1223396	32.07	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	47716	8.08	ng/ul	0.00
57) Fluorene-d10	15.89	176	1029565	32.70	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	202768	31.08	ng/ul	0.00
70) Anthracene-d10	17.74	188	1583965	32.30	ng/ul	0.00
76) Pyrene-d10	20.01	212	1919435	32.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	1926074	33.64	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.34	163	55750	1.71 ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
Data File : BG024271.D
Acq On : 11 Oct 2016 18:57
Operator : UM/SJ
Sample : H5113-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDP72

Quant Time: Oct 12 04:50:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 04:50:43 2016
Response via : Initial Calibration

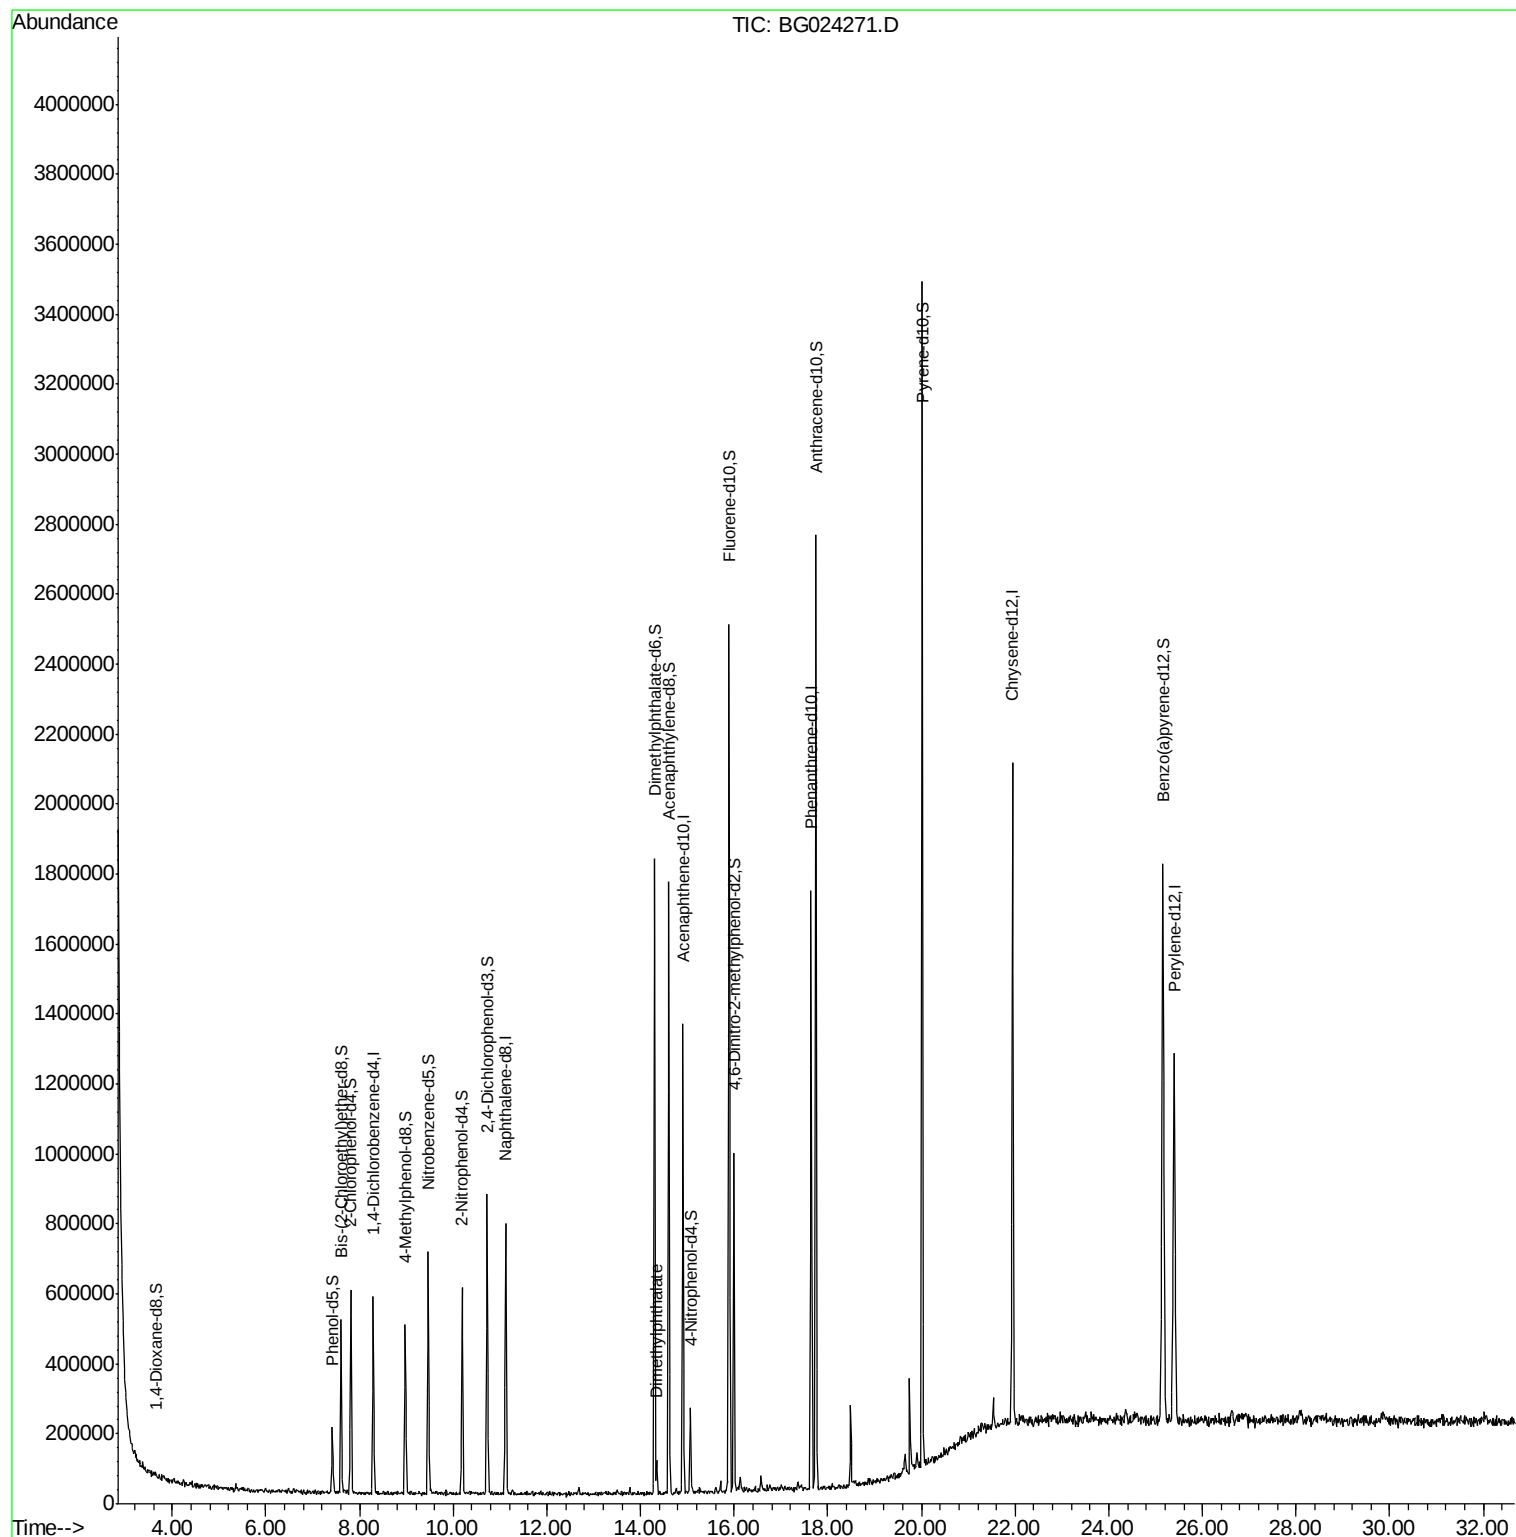

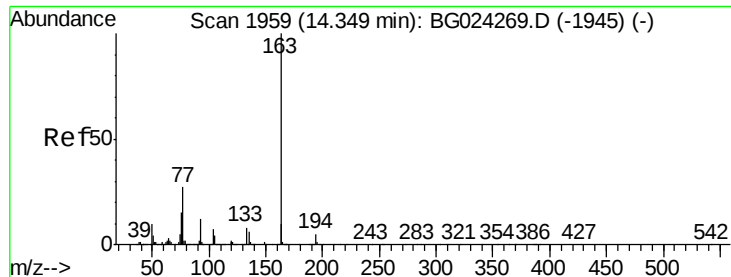

#44

Dimethylphthalate

Concen: 1.71 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. -0.01 min

Lab File: BG024271.D

Acq: 11 Oct 2016 18:57

Instrument :

BNA_G

ClientSampleId :

BDP72


Tgt Ion:163 Resp: 55750

Ion Ratio Lower Upper

163 100

194 1.7 3.4 5.0#

164 6.9 9.0 13.4#

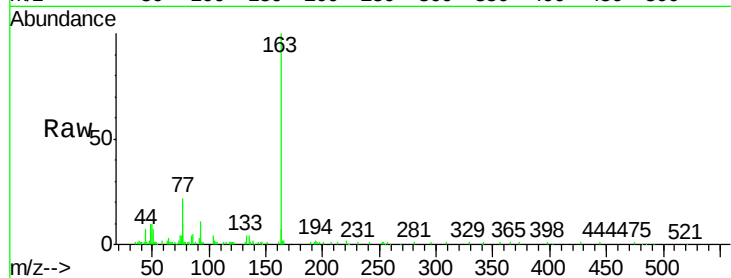

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

