

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
 Data File : BG024281.D
 Acq On : 12 Oct 2016 1:22
 Operator : UM/SJ
 Sample : H5113-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDP62

Quant Time: Oct 12 04:52:22 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 04:50:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	160025	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	651297	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	500154	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.74	188	1432322	20.00	ng/ul	0.09
75) Chrysene-d12	21.94	240	1227242	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1253215	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	15009	4.45	ng/uL	0.00
5) Phenol-d5	7.41	99	334988	22.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	223360	22.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	240613	23.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	262071	21.71	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	122832	26.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	142115	27.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	269478	23.93	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	248572	21.01	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	950062	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1110148	27.75	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	168557	27.22	ng/ul	0.00
57) Fluorene-d10	15.89	176	911913	27.62	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.08	200	320	0.04	ng/ul	0.08
70) Anthracene-d10	17.74	188	1432624	22.14	ng/ul	0.00
76) Pyrene-d10	20.01	212	1681949	29.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	1639420	29.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.35	163	806266	23.55	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101116\
Data File : BG024281.D
Acq On : 12 Oct 2016 1:22
Operator : UM/SJ
Sample : H5113-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDP62

Quant Time: Oct 12 04:52:22 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 04:50:43 2016
Response via : Initial Calibration

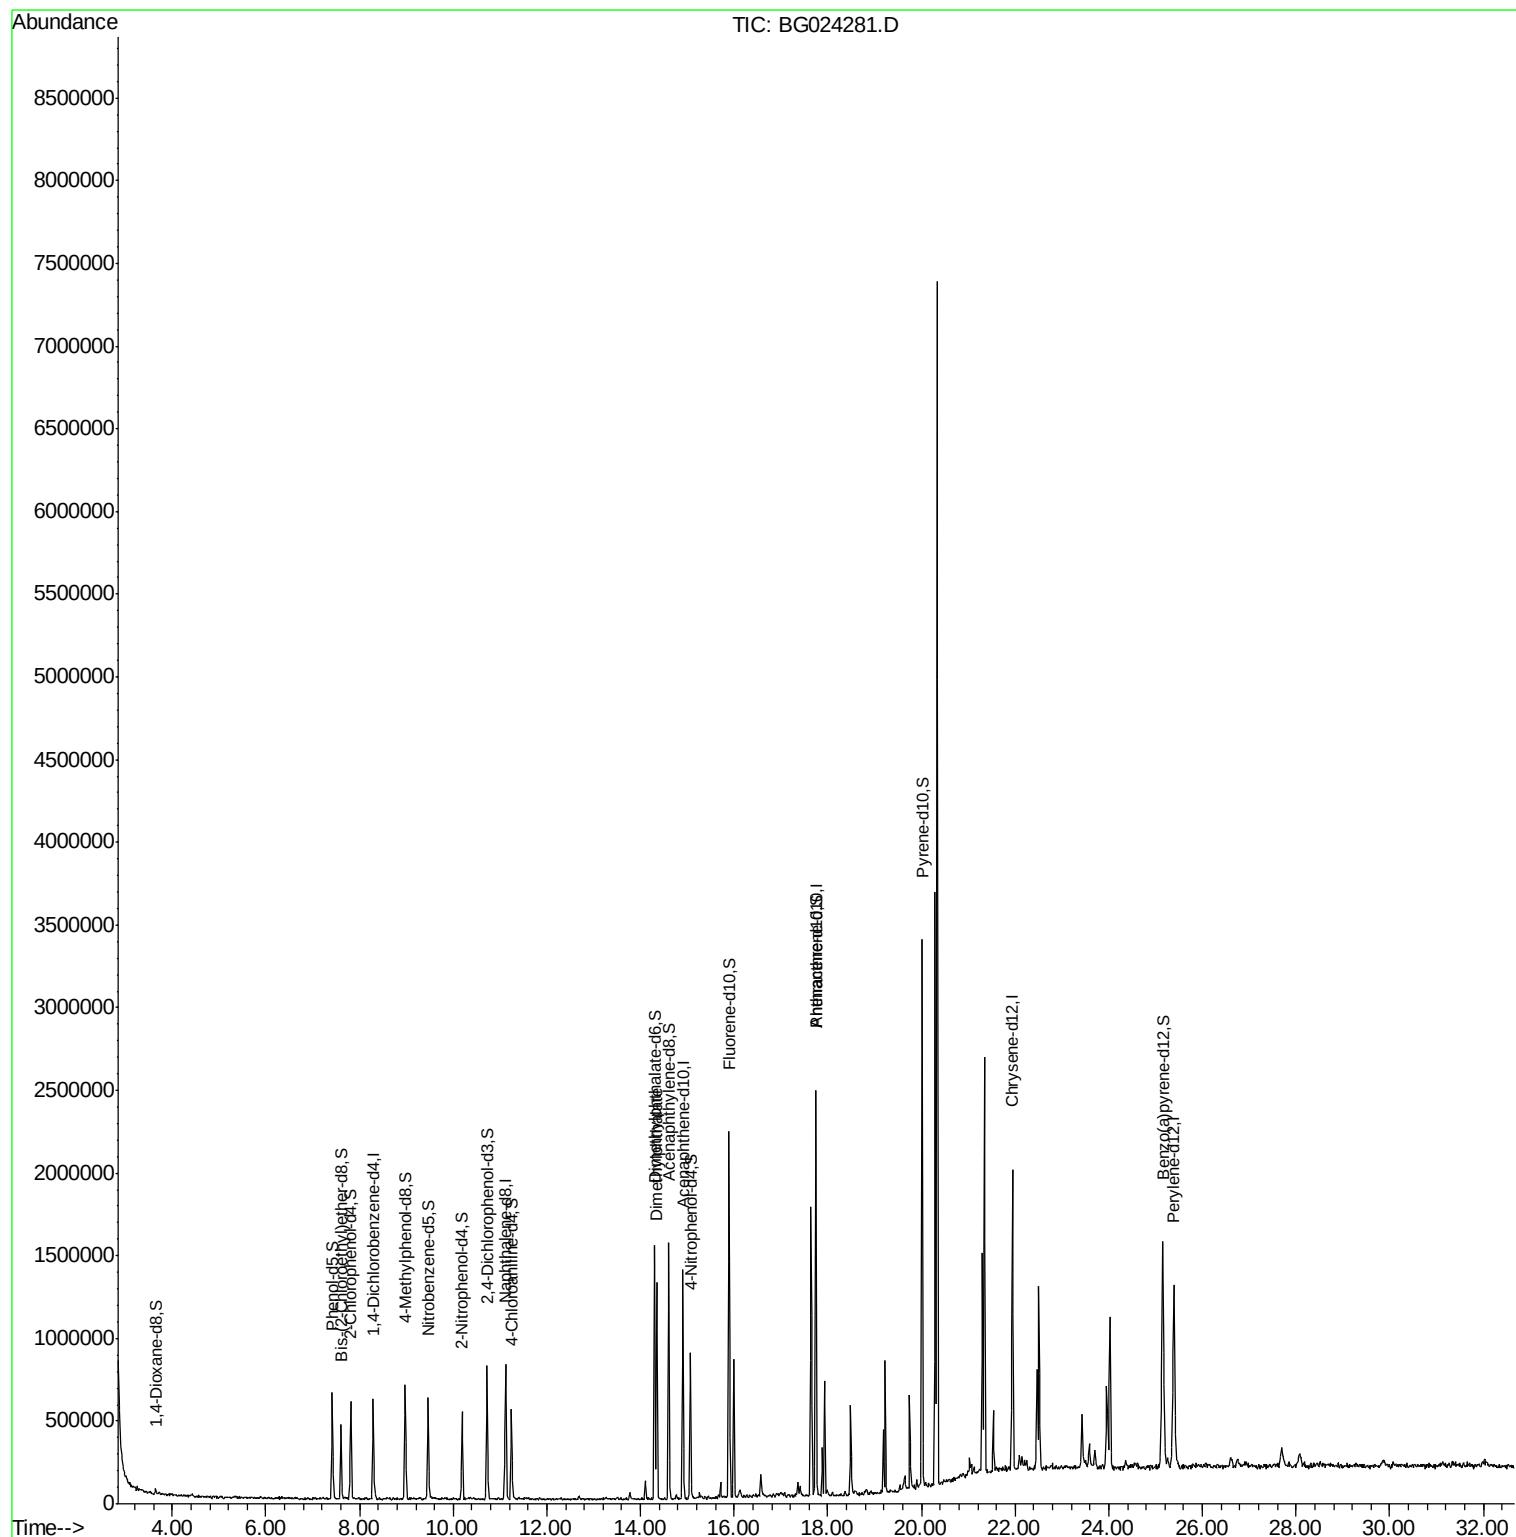

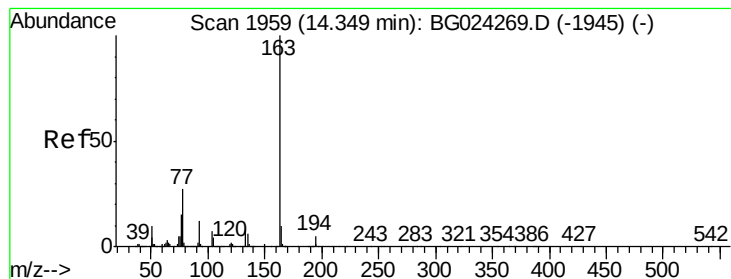

#44

Dimethylphthalate

Concen: 23.55 ng/ul

RT: 14.35 min Scan# 1959

Delta R.T. -0.00 min

Lab File: BG024281.D

Acq: 12 Oct 2016 1:22

Instrument :

BNA_G

ClientSampleId :

BDP62


Tgt Ion:163 Resp: 806266

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 10.8 9.0 13.4

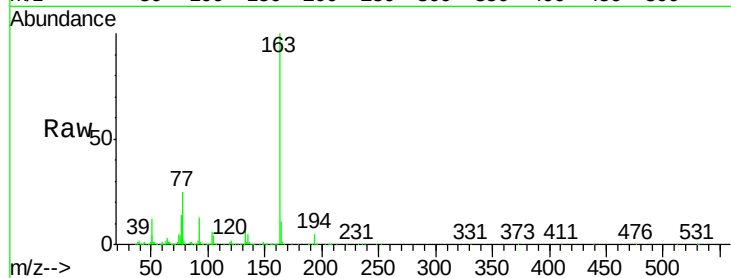

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

