

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101116\
 Data File : BG024278.D
 Acq On : 11 Oct 2016 23:27
 Operator : UM/SJ
 Sample : H5113-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDP53

Quant Time: Oct 12 04:51:54 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 12 04:50:43 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	140012	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	609933	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	496304	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1094701	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1230775	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1255814	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	17088	5.80	ng/uL	0.00
5) Phenol-d5	7.42	99	392979	30.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	265487	30.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	280675	31.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	322484	30.54	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	147457	34.07	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	168610	34.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	325773	30.89	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	295208	26.64	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1208575	34.88	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1358241	34.22	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	218519	35.56	ng/ul	0.00
57) Fluorene-d10	15.89	176	1117940	34.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	236782	35.99	ng/ul	0.00
70) Anthracene-d10	17.74	188	1778515	35.97	ng/ul	0.00
76) Pyrene-d10	20.01	212	2101543	36.58	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	2095402	37.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.35	163	768849	22.63	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101116\
Data File : BG024278.D
Acq On : 11 Oct 2016 23:27
Operator : UM/SJ
Sample : H5113-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDP53

Quant Time: Oct 12 04:51:54 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 12 04:50:43 2016
Response via : Initial Calibration

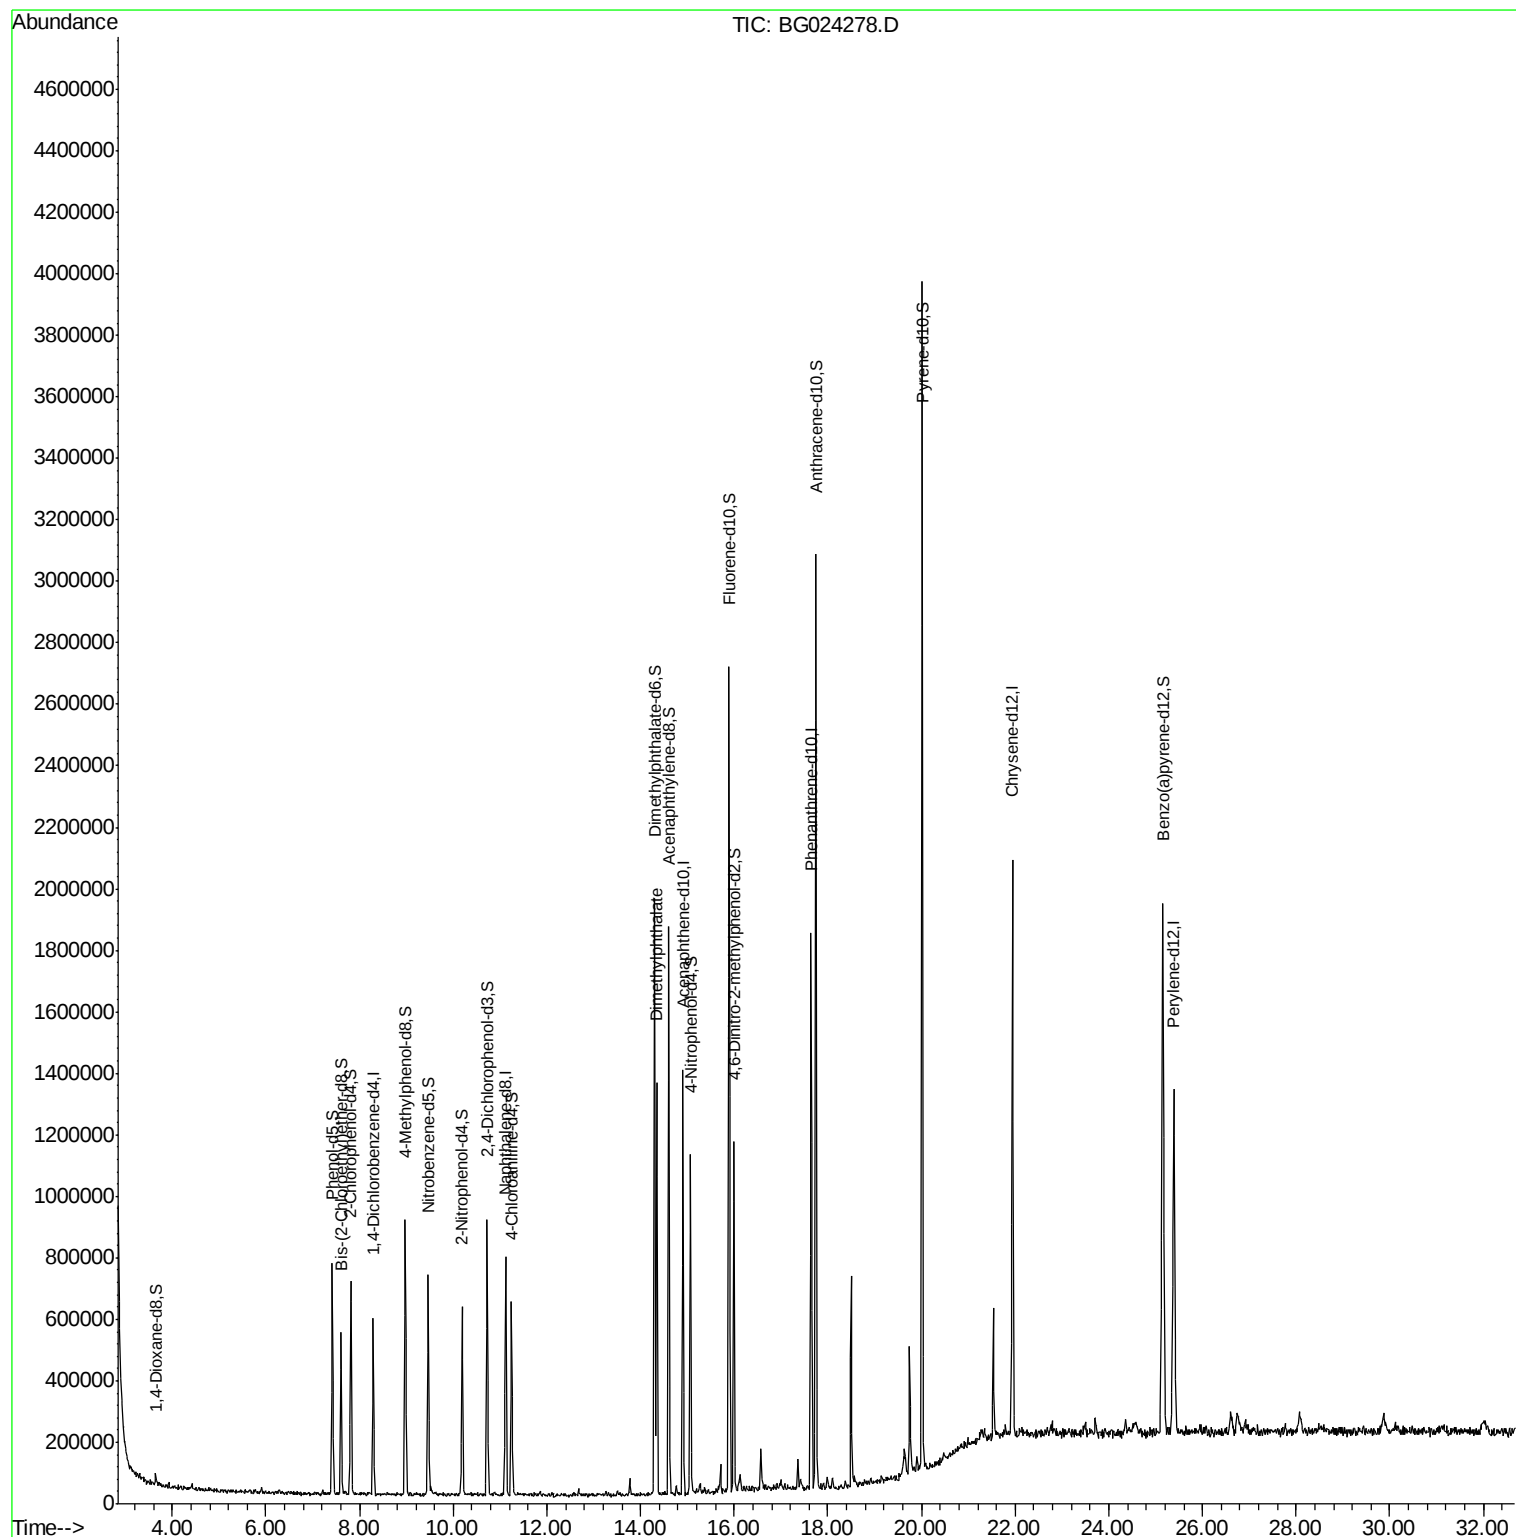

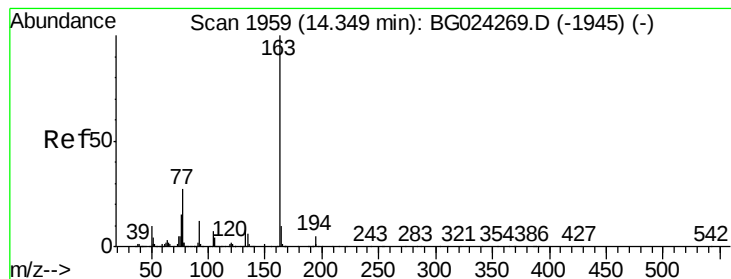

#44

Dimethylphthalate

Concen: 22.63 ng/ul

RT: 14.35 min Scan# 1959

Delta R.T. -0.00 min

Lab File: BG024278.D

Acq: 11 Oct 2016 23:27

Instrument :

BNA_G

ClientSampleId :

BDP53


Tot Ion:163 Resp: 768849

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.0

164 10.3 9.0 13.4

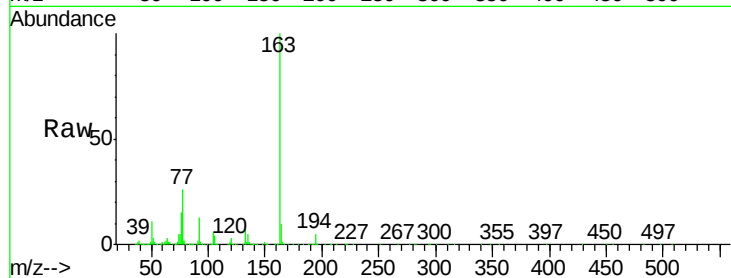

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

