

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101117\
 Data File : BG029159.D
 Acq On : 11 Oct 2017 4:42
 Operator : SJ/JU
 Sample : I5668-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB3G3

Quant Time: Oct 11 07:03:07 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101117.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 11 04:24:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.22	152	46225	20.00	ng/ul	0.00
2) Naphthalene-d8	11.04	136	204069	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.82	164	137673	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.57	188	322785	20.00	ng/ul	0.00
18) Chrysene-d12	21.84	240	348721	20.00	ng/ul	0.00
23) Perylene-d12	25.19	264	350689	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.65	165	31882	8.17	ng/ul	0.00
7) Acenaphthylene-d8	14.53	160	304887	22.09	ng/ul	0.00
10) Fluorene-d10	15.81	176	231116	21.34	ng/ul	0.00
15) Anthracene-d10	17.66	188	340006	21.31	ng/ul	0.00
19) Pyrene-d10	19.94	212	415231	22.66	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.96	264	384501	21.92	ng/ul	0.00
Target Compounds				Qvalue		
4) Naphthalene	11.08	128	11151	1.040	ng/ul#	87
9) Acenaphthene	14.89	153	11262	1.213	ng/ul	95
11) Fluorene	15.87	166	12250	1.145	ng/ul	96
14) Phenanthrene	17.61	178	225036	12.871	ng/ul	98
16) Anthracene	17.70	178	45802	2.555	ng/ul	99
17) Fluoranthene	19.60	202	380012	18.470	ng/ul	98
20) Pyrene	19.96	202	330906	15.651	ng/ul	99
21) Benzo(a)anthracene	21.83	228	197978	9.318	ng/ul	98
22) Chrysene	21.89	228	181495	9.464	ng/ul	95
24) Benzo(b)fluoranthene	24.13	252	259526	12.010	ng/ul#	96
25) Benzo(k)fluoranthene	24.19	252	70979	3.334	ng/ul	98
27) Benzo(a)pyrene	25.03	252	158519	7.516	ng/ul	99
28) Indeno(1,2,3-cd)pyrene	29.02	276	84680	4.213	ng/ul	94
30) Benzo(g,h,i)perylene	30.21	276	24469	1.746	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101117\
Data File : BG029159.D
Acq On : 11 Oct 2017 4:42
Operator : SJ/JU
Sample : I5668-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB3G3

Quant Time: Oct 11 07:03:07 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG101117.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 11 04:24:22 2017
Response via : Initial Calibration

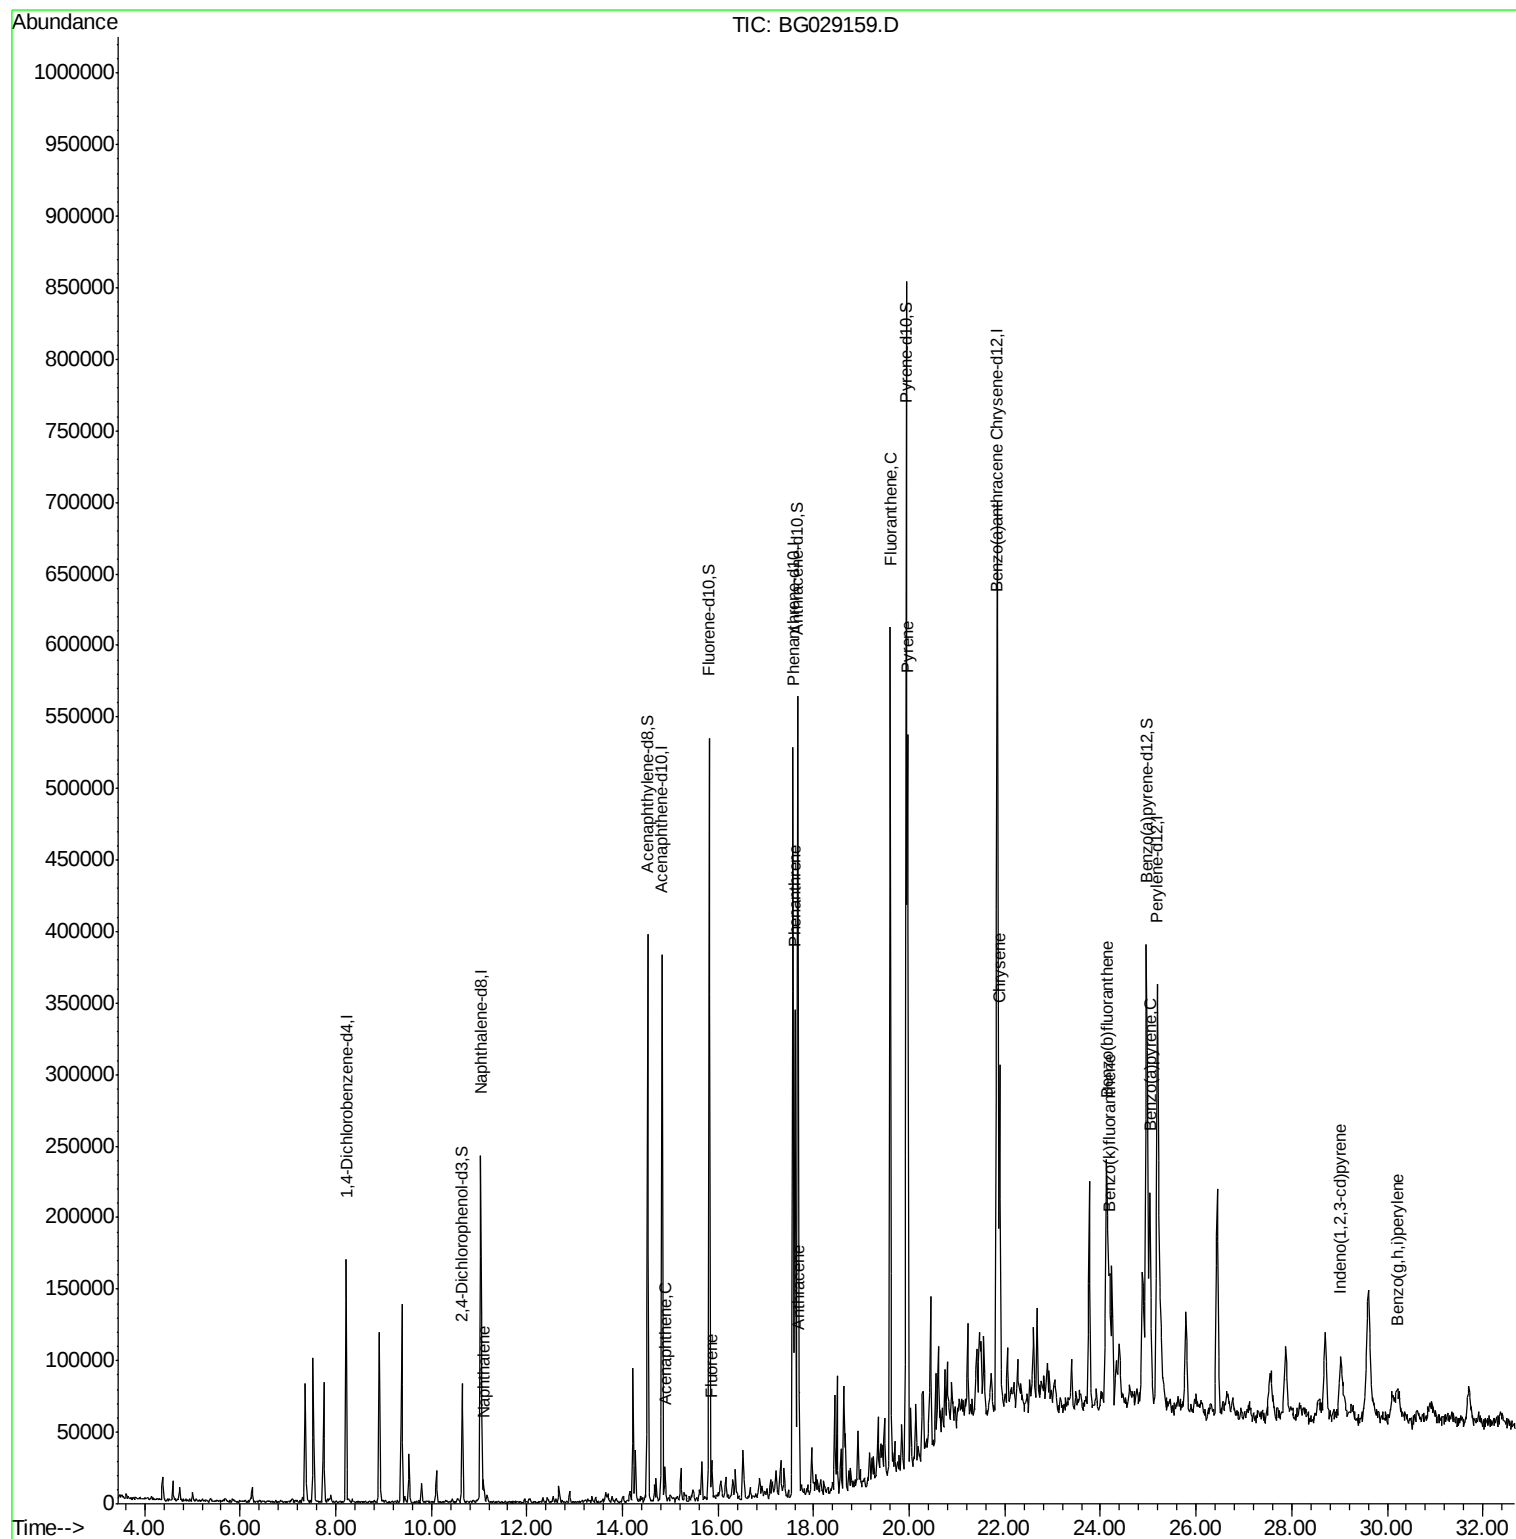

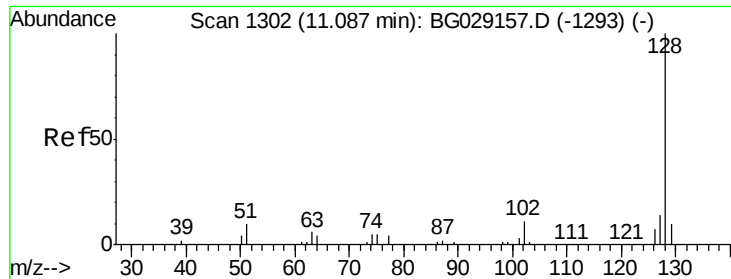

#4

Naphthalene

Concen: 1.040 ng/ul

RT: 11.08 min Scan# 1301

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampleId :

CB3G3


Tgt Ion:128 Resp: 11151

Ion Ratio Lower Upper

128 100

129 7.6 9.0 13.4#




127 19.8 10.6 15.8#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

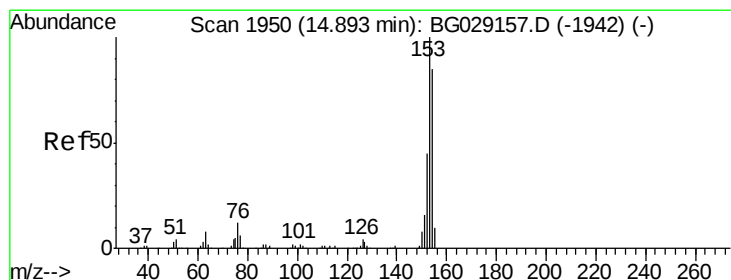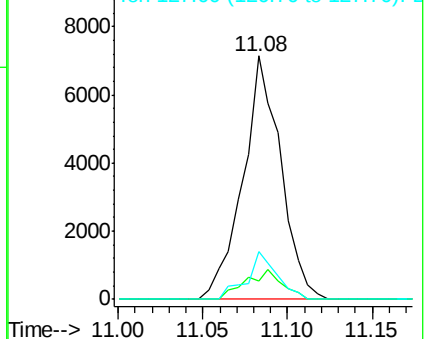

#9

Acenaphthene

Concen: 1.213 ng/ul

RT: 14.89 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:153 Resp: 11262

Ion Ratio Lower Upper

153 100

152 48.4 36.2 54.4



154 80.5 68.4 102.6




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

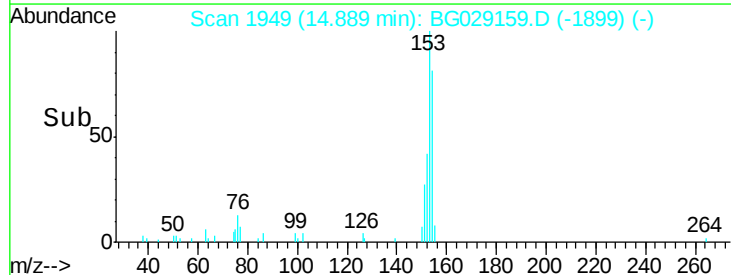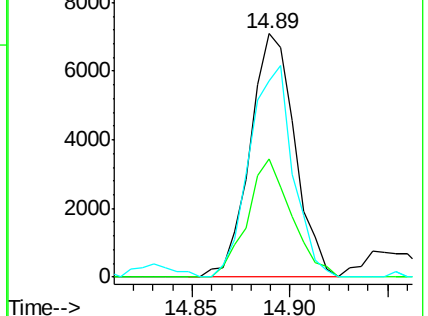



#11

Fluorene

Concen: 1.145 ng/ul

RT: 15.87 min Scan# 2116

Delta R.T. 0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampled :

CB3G3


Tgt Ion:166 Resp: 12250

Ion Ratio Lower Upper

166 100

165 103.2 79.4 119.0




167 11.1 10.2 15.4

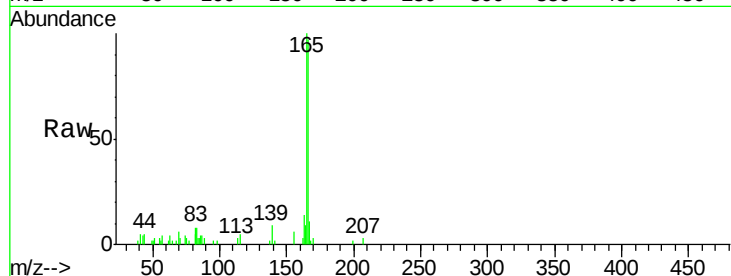

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

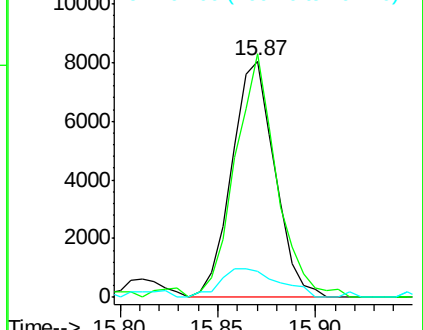

#14

Phenanthrene

Concen: 12.871 ng/ul

RT: 17.61 min Scan# 2412

Delta R.T. 0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:178 Resp: 225036

Ion Ratio Lower Upper

178 100

179 16.2 12.2 18.2



176 19.9 15.0 22.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

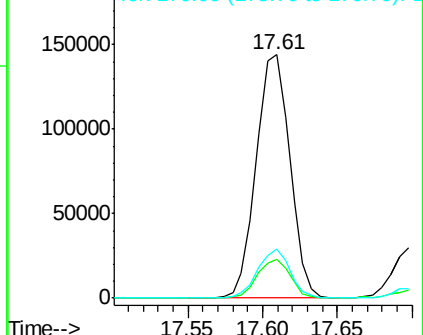



#16

Anthracene

Concen: 2.555 ng/ul

RT: 17.70 min Scan# 2427

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampleId :

CB3G3


Tgt Ion:178 Resp: 45802

Ion Ratio Lower Upper

178 100

179 14.9 12.5 18.7




176 19.3 15.7 23.5

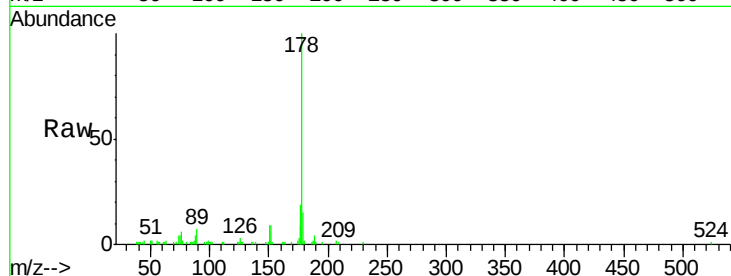

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

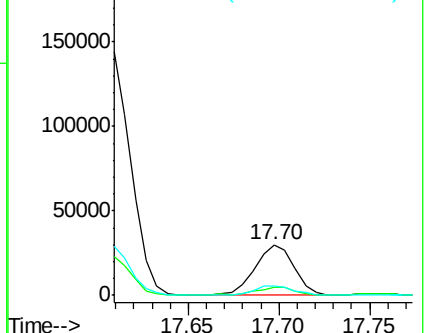

#17

Fluoranthene

Concen: 18.470 ng/ul

RT: 19.60 min Scan# 2751

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:202 Resp: 380012

Ion Ratio Lower Upper

202 100

101 7.8 5.6 8.4



100 6.1 4.7 7.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

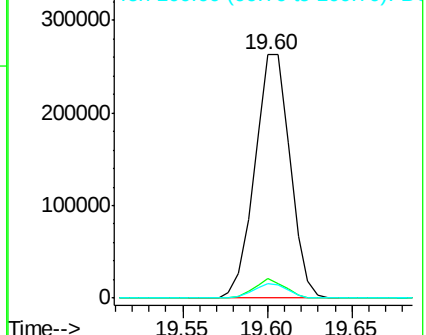







#20
 Pyrene
 Concen: 15.651 ng/ul
 RT: 19.96 min Scan# 2813
 Delta R.T. 0.00 min
 Lab File: BG029159.D
 Acq: 11 Oct 2017 4:42

Instrument :
 BNA_G
 ClientSampleId :
 CB3G3

Tgt Ion:	202	Resp:	330906
Ion	Ratio	Lower	Upper
202	100		
101	8.2	6.5	9.7
100	6.4	5.5	8.3

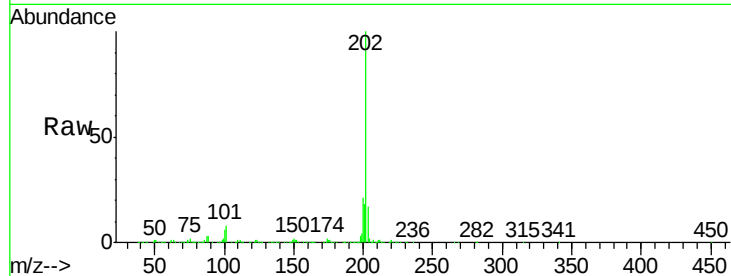


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

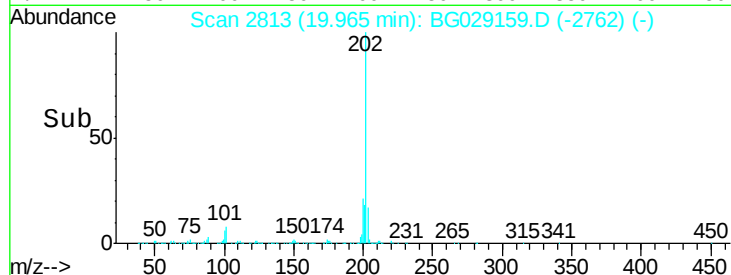
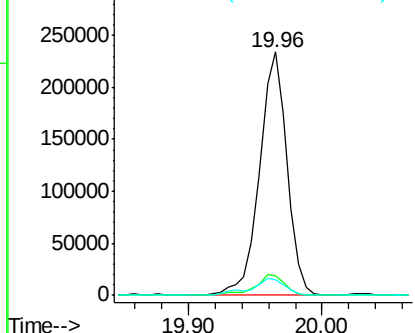



#21
 Benzo(a)anthracene
 Concen: 9.318 ng/ul
 RT: 21.83 min Scan# 3130
 Delta R.T. 0.00 min
 Lab File: BG029159.D
 Acq: 11 Oct 2017 4:42

Tgt Ion:	228	Resp:	197978
Ion	Ratio	Lower	Upper
228	100		
229	21.5	15.8	23.8
226	27.1	21.6	32.4

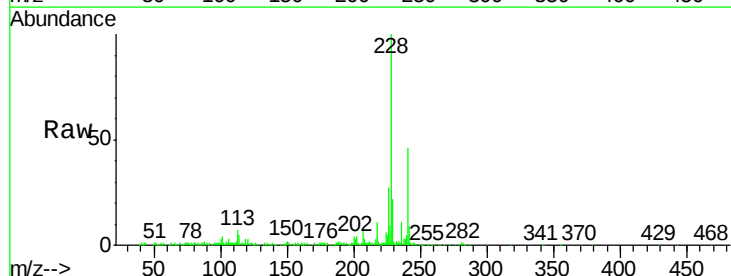

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E

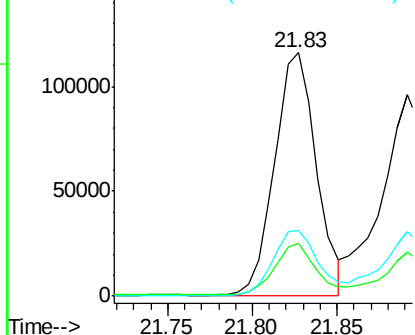

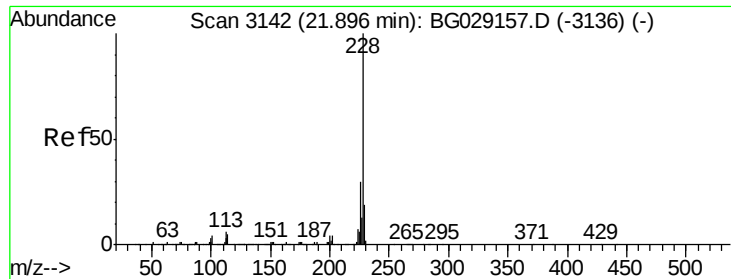

#22

Chrysene

Concen: 9.464 ng/ul

RT: 21.89 min Scan# 3141

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampleId :

CB3G3


Tgt Ion:228 Resp: 181495

Ion Ratio Lower Upper

228 100

226 32.0 23.4 35.0




229 21.7 15.7 23.5

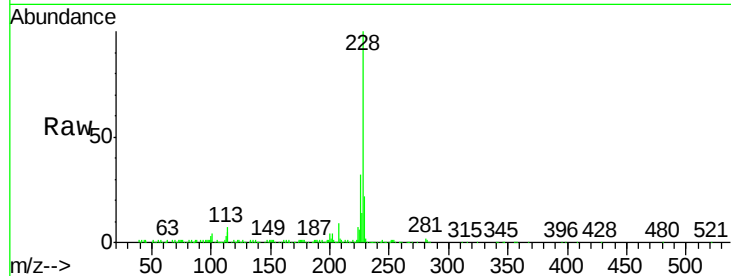

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

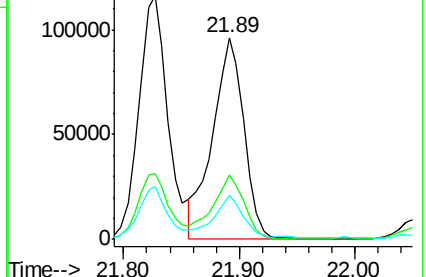

#24

Benzo(b)fluoranthene

Concen: 12.010 ng/ul

RT: 24.13 min Scan# 3522

Delta R.T. 0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:252 Resp: 259526

Ion Ratio Lower Upper

252 100

253 23.6 17.6 26.4



125 7.4 4.5 6.7#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

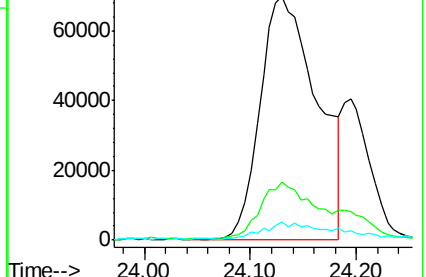

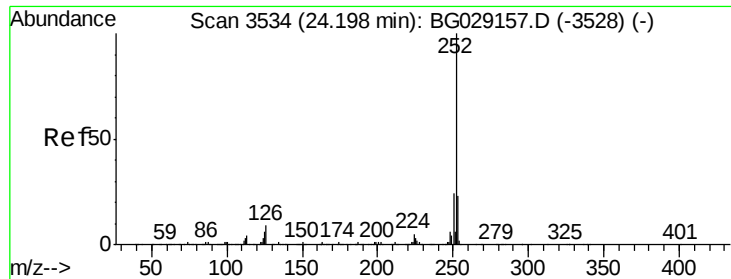

#25

Benzo(k)fluoranthene

Concen: 3.334 ng/ul

RT: 24.19 min Scan# 3533

Delta R.T. -0.00 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampleId :

CB3G3


Tgt Ion:252 Resp: 70979

Ion Ratio Lower Upper

252 100

253 20.1 16.8 25.2




125 6.9 5.1 7.7

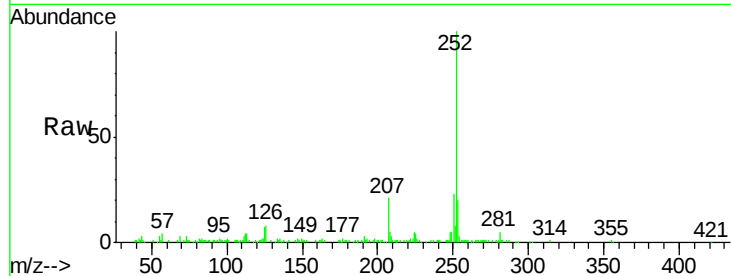

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

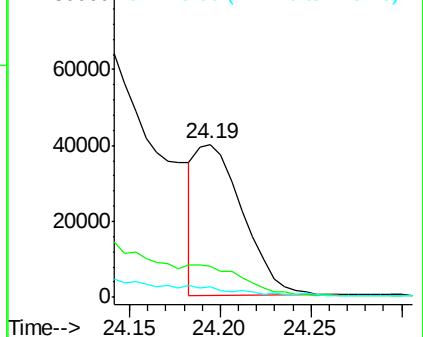

#27

Benzo(a)pyrene

Concen: 7.516 ng/ul

RT: 25.03 min Scan# 3676

Delta R.T. -0.01 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:252 Resp: 158519

Ion Ratio Lower Upper

252 100

253 21.8 17.6 26.4



125 5.9 5.4 8.2




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

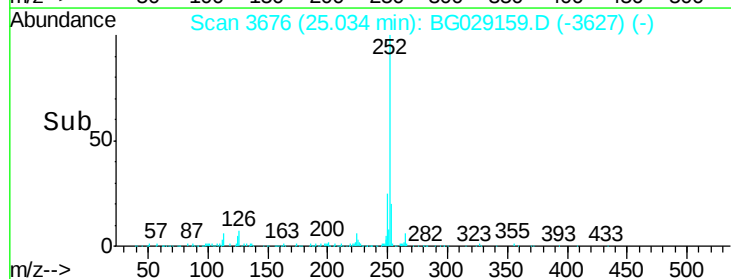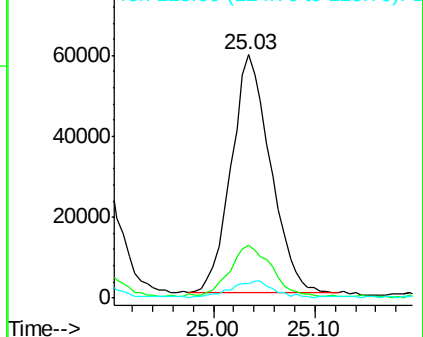



#28

Indeno(1,2,3-cd)pyrene

Concen: 4.213 ng/ul

RT: 29.02 min Scan# 4355

Delta R.T. -0.02 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42

Instrument :

BNA_G

ClientSampleId :

CB3G3


Tgt Ion:276 Resp: 84680

Ion Ratio Lower Upper

276 100

138 12.7 9.5 14.3




277 26.8 18.1 27.1

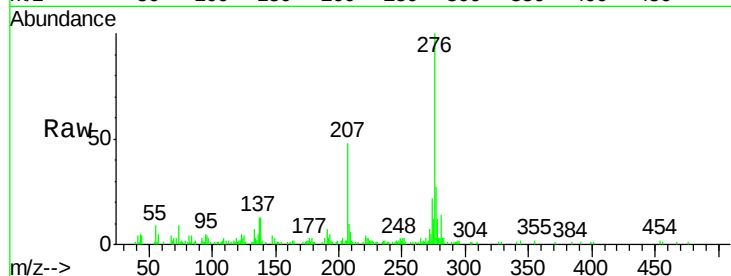

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

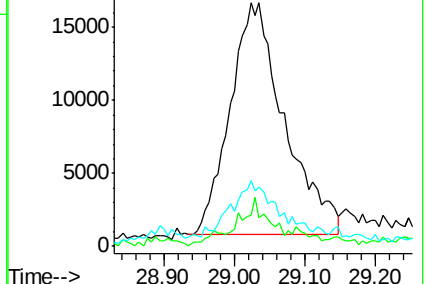

#30

Benzo(g,h,i)perylene

Concen: 1.746 ng/ul

RT: 30.21 min Scan# 4557

Delta R.T. -0.03 min

Lab File: BG029159.D

Acq: 11 Oct 2017 4:42


Tgt Ion:276 Resp: 24469

Ion Ratio Lower Upper

276 100

138 11.8 9.3 13.9

277 21.4 17.9 26.9



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

