



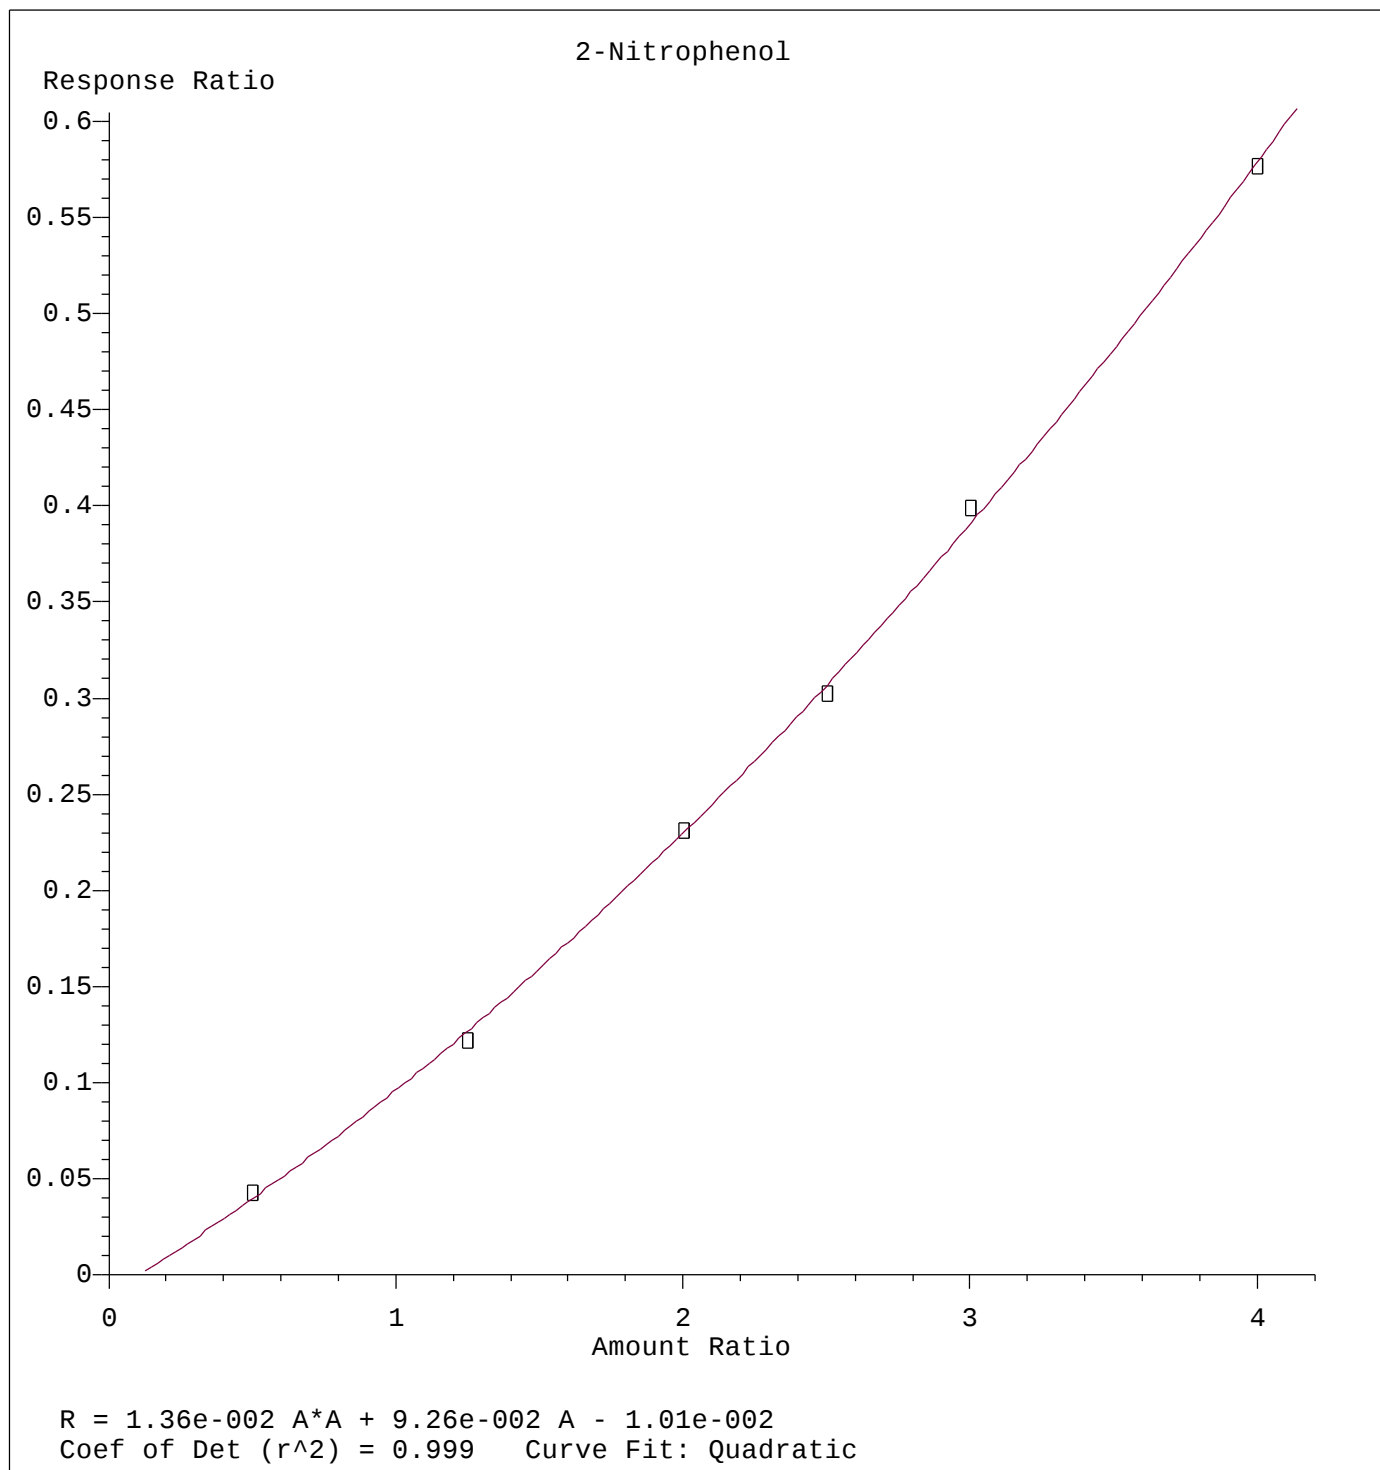

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Calibration Table Last Updated: Thu Oct 11 13:59:58 2018

2-Nitroaniline

Response Ratio

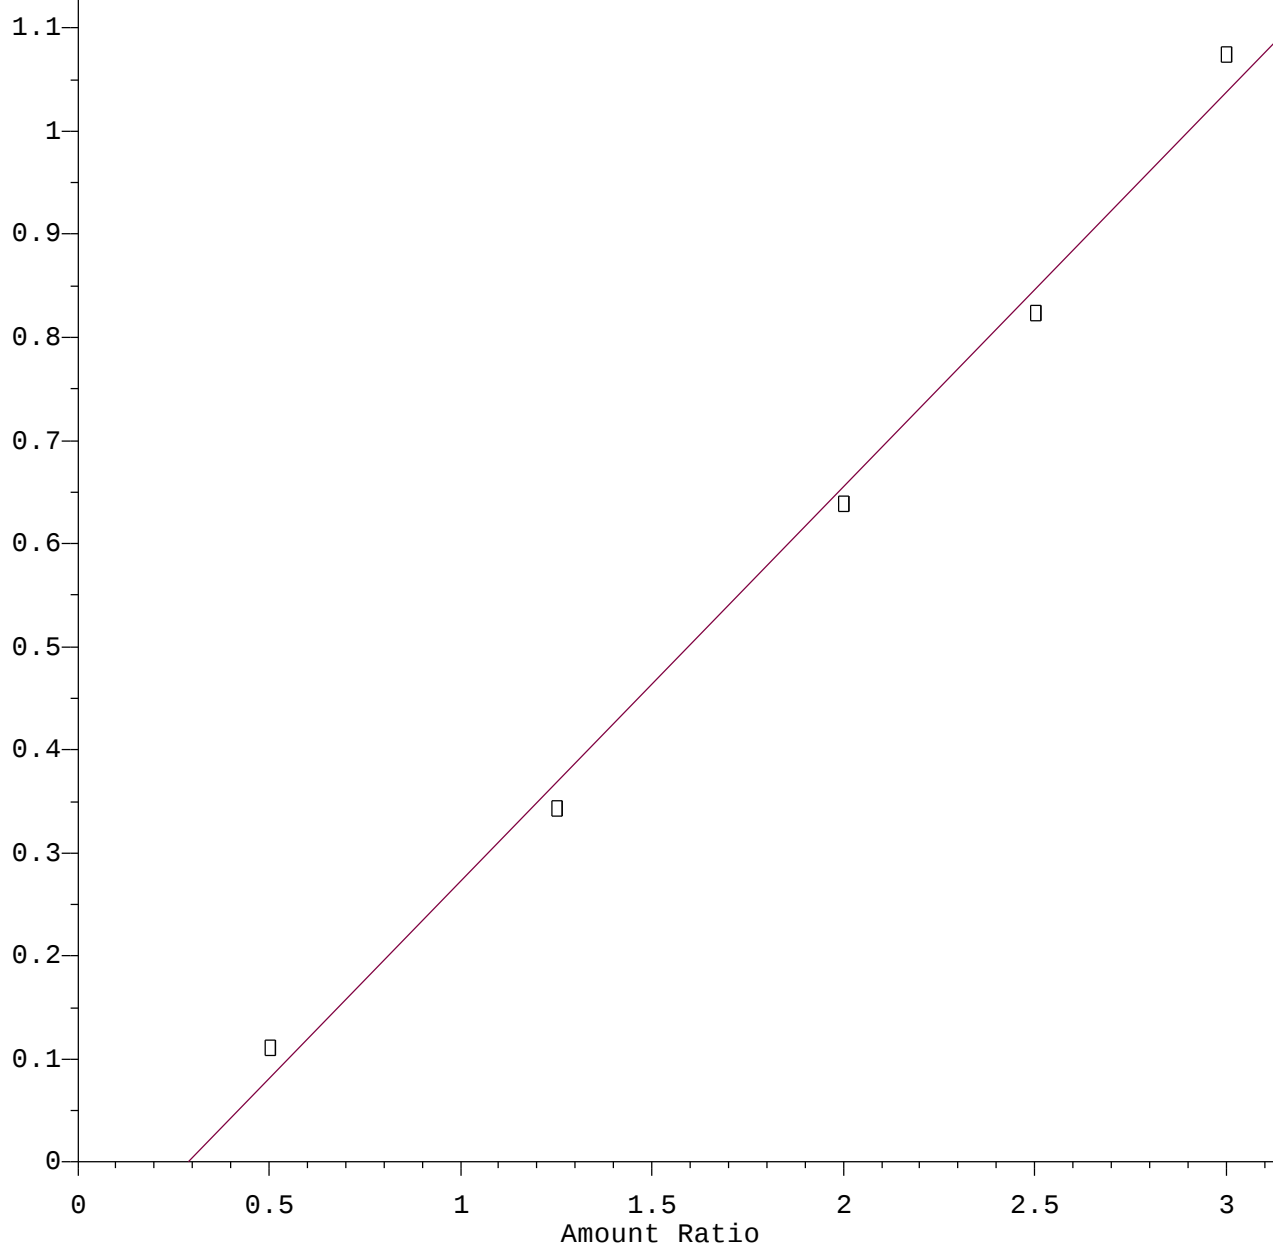


Resp Ratio = $3.83 \times 10^{-1} \times \text{Amt} - 1.10 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Calibration Table Last Updated: Thu Oct 11 13:59:58 2018

2,6-Dinitrotoluene

Response Ratio

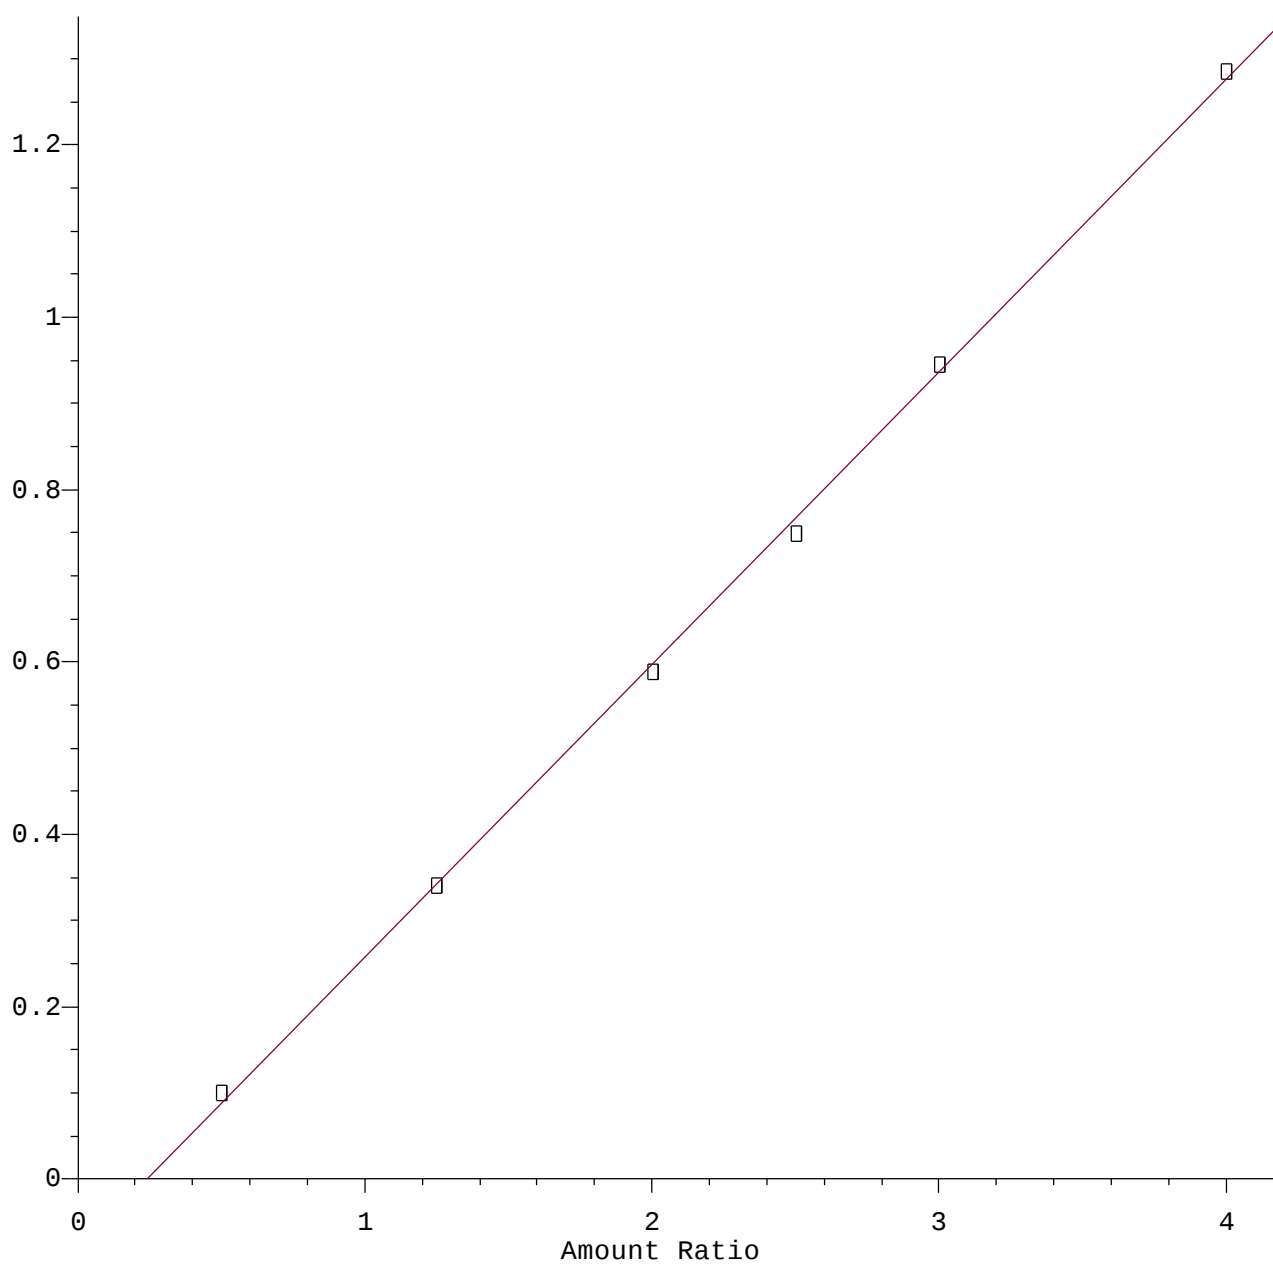


Resp Ratio = $3.39 \times 10^{-1} \times \text{Amt} - 8.16 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Calibration Table Last Updated: Thu Oct 11 13:59:58 2018

2,4-Dinitrotoluene


Response Ratio

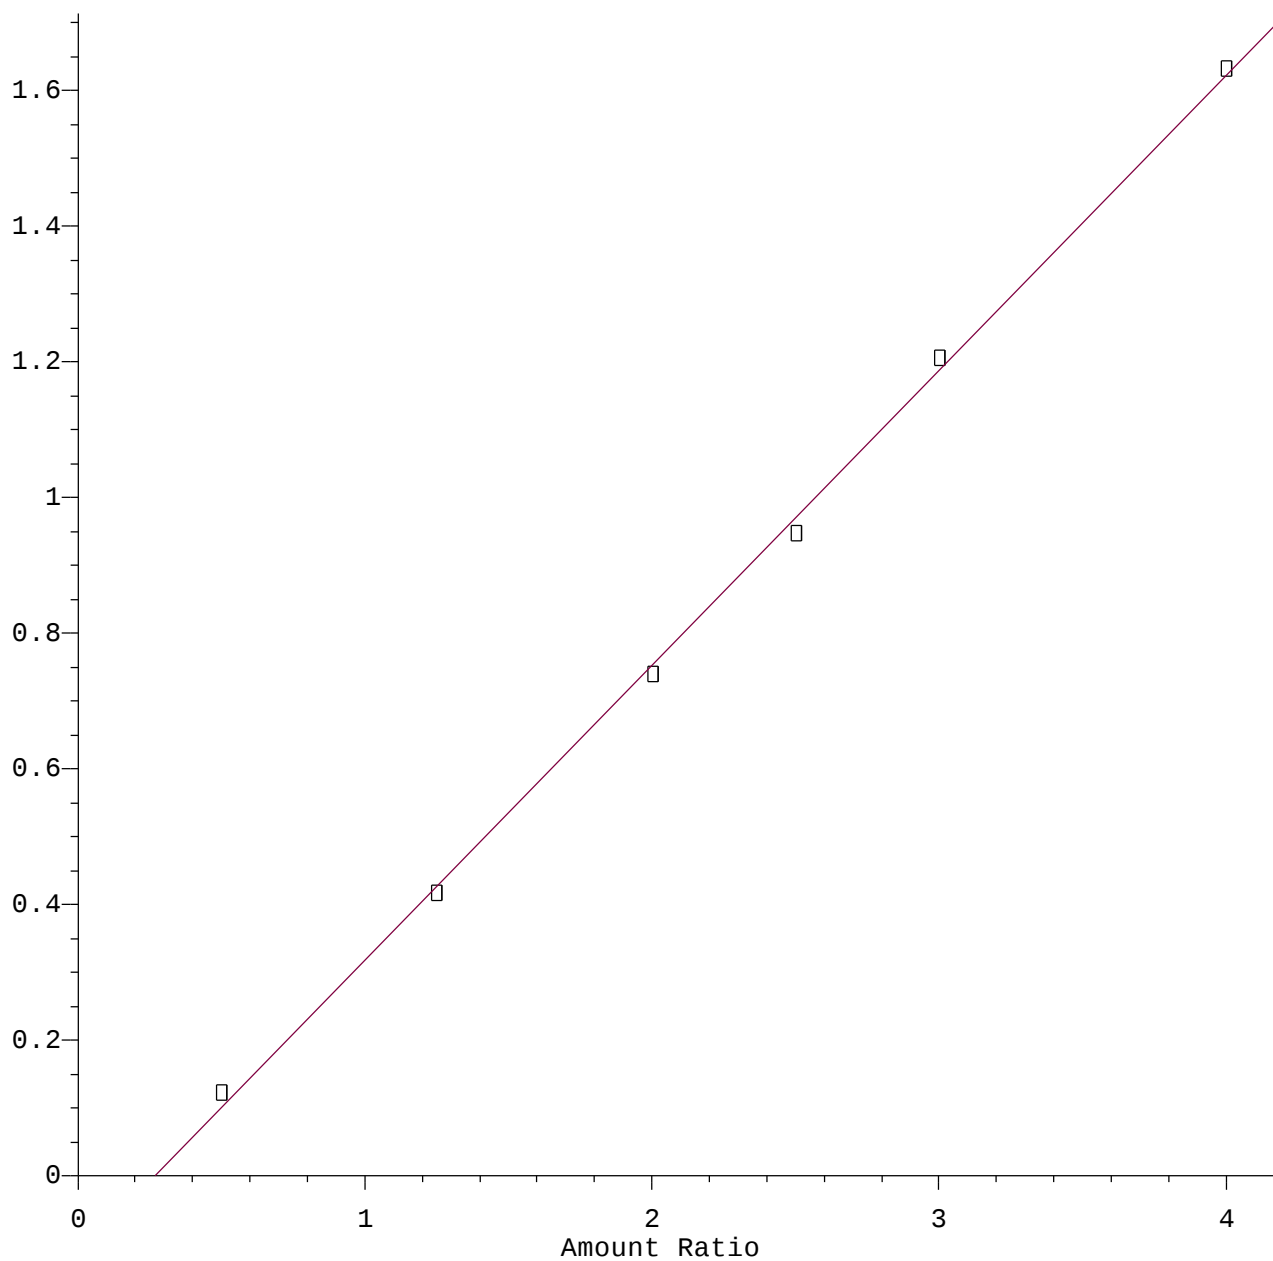

Resp Ratio = $4.35 \times 10^{-1} \times \text{Amt} - 1.16 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Calibration Table Last Updated: Thu Oct 11 13:59:58 2018

4,6-Dinitro-2-methylphenol

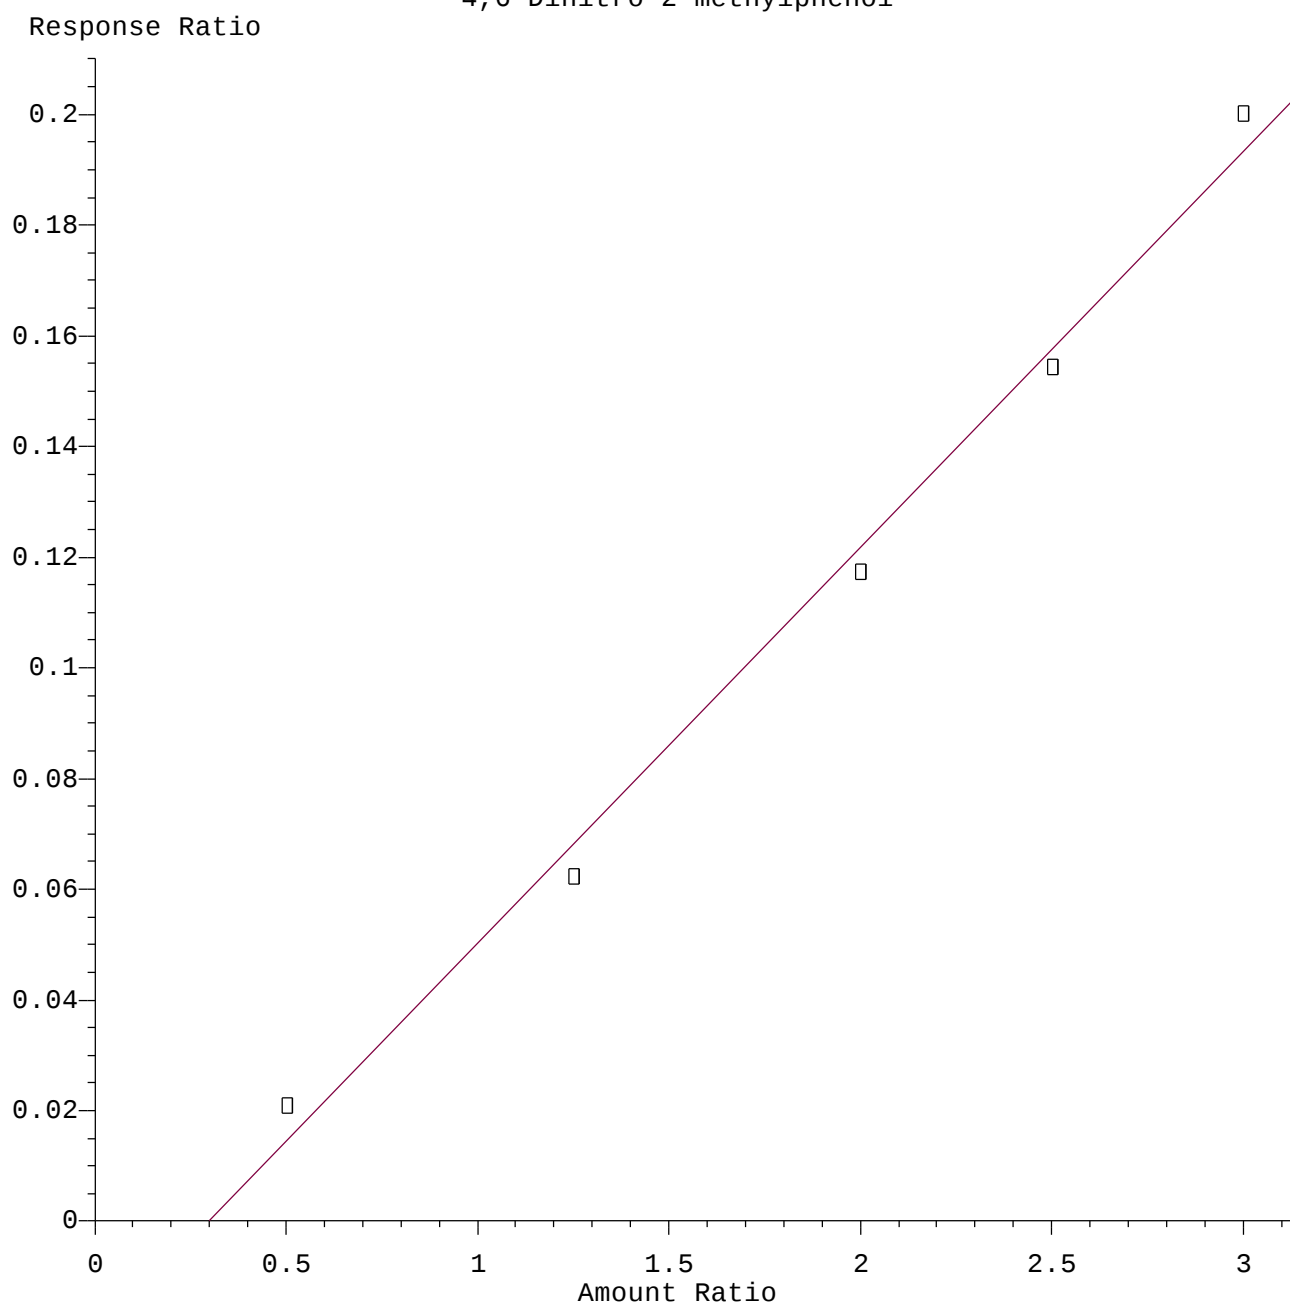

Resp Ratio = $7.15 \times 10^{-2} \times \text{Amt} - 2.12 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
Calibration Table Last Updated: Thu Oct 11 13:59:58 2018