
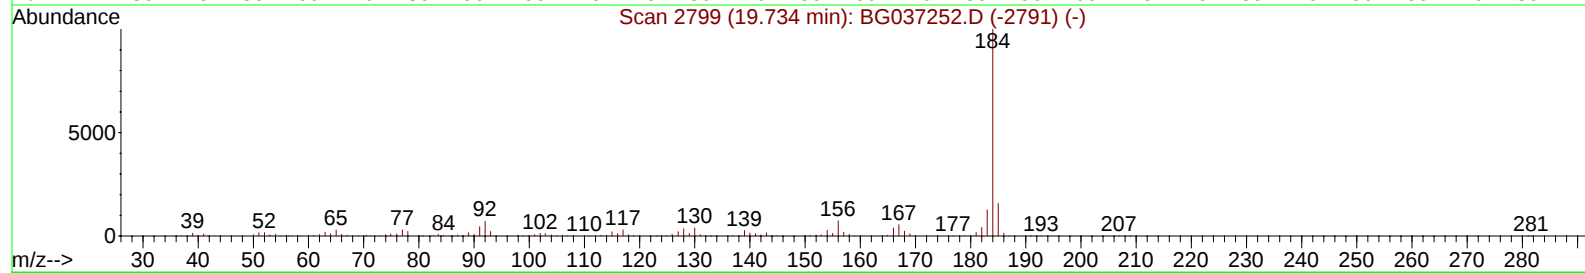
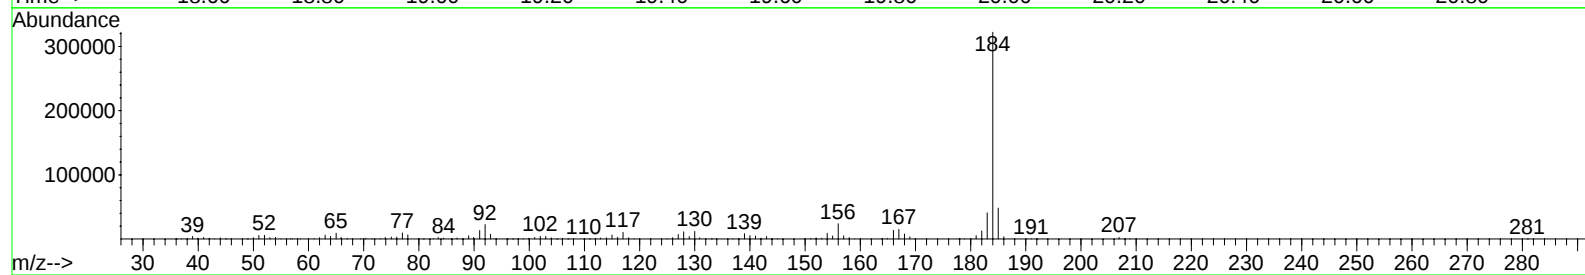


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\
Data File : BG037248.D
Acq On : 11 Oct 2018 8:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 14:57:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

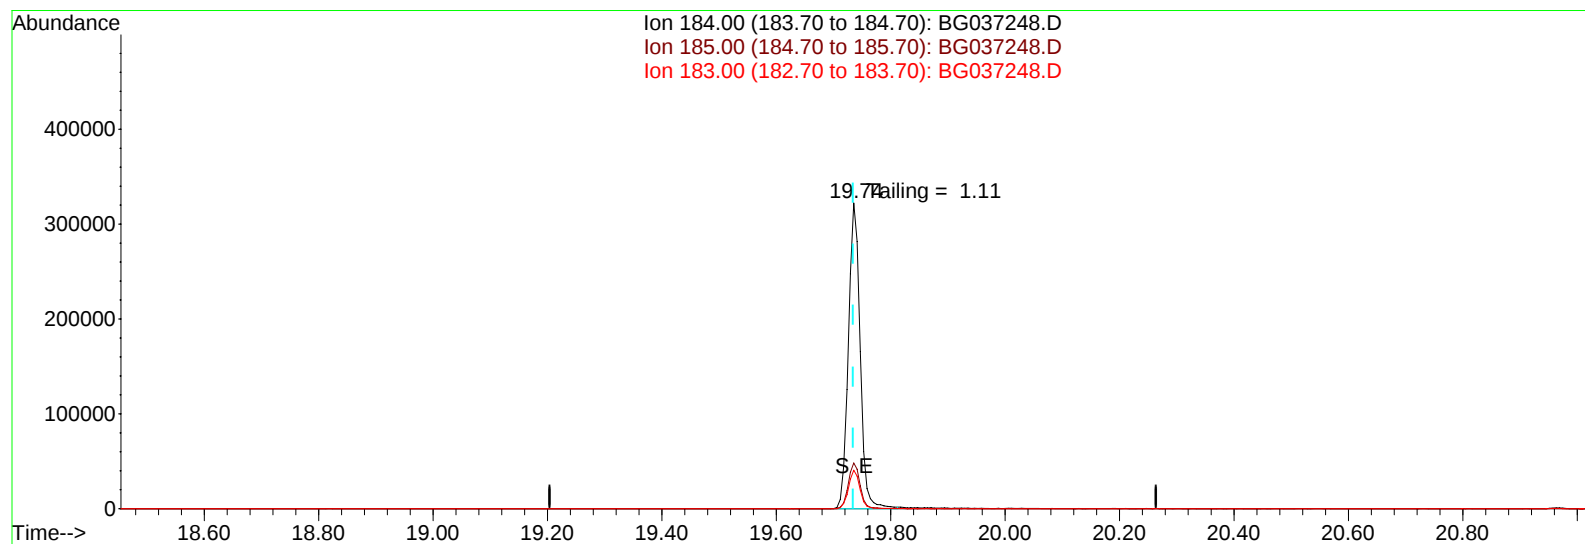

TIC: BG037248.D

(77) Benzidine




19.735min (+0.001) 26167.35ng

response 466489

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.98
183.00	12.70	12.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\
Data File : BG037248.D
Acq On : 11 Oct 2018 8:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 14:57:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

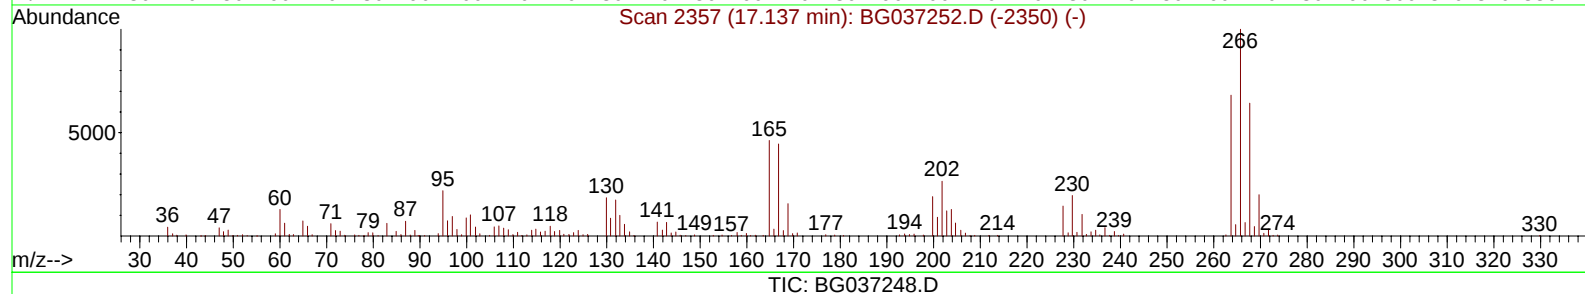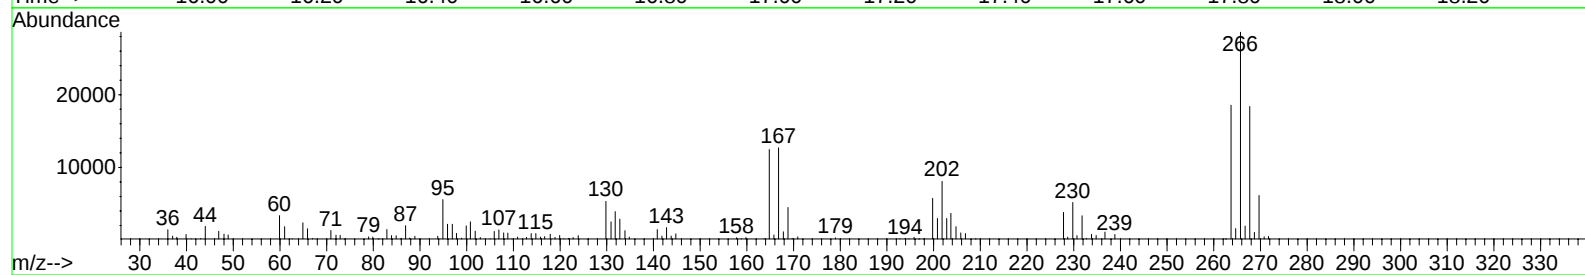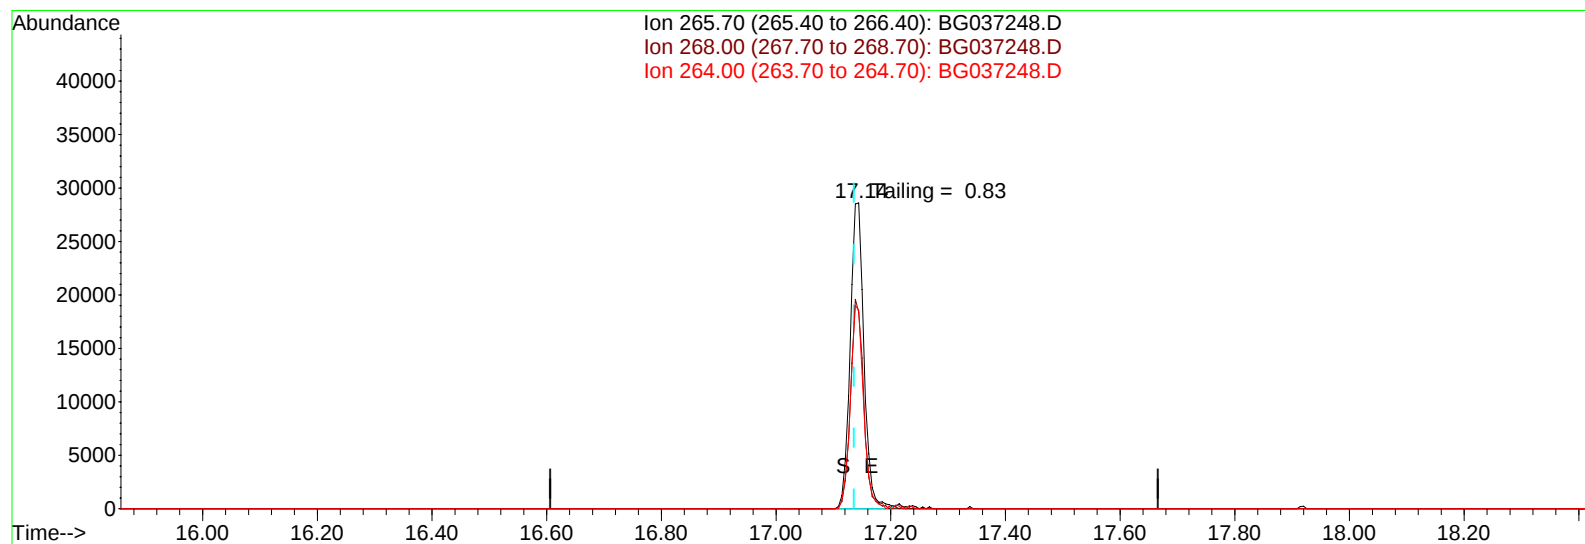

(70) Pentachlorophenol (C)

17.144min (+0.008) 19189.61ng

response 47796

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	67.99
264.00	73.60	70.48
0.00	0.00	0.00