
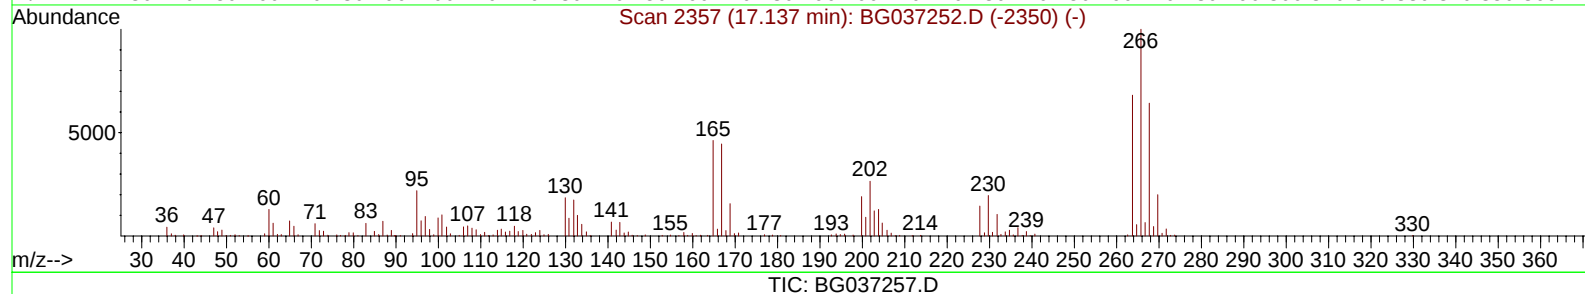
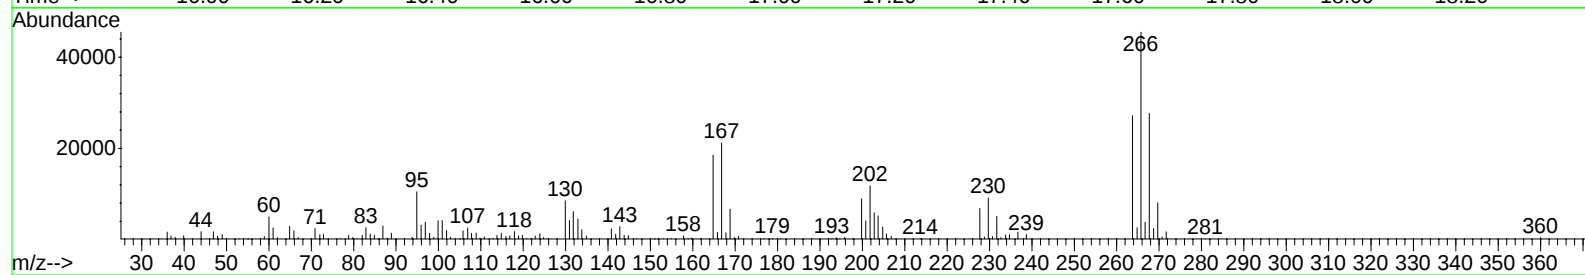


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\
Data File : BG037257.D
Acq On : 11 Oct 2018 14:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 17:03:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

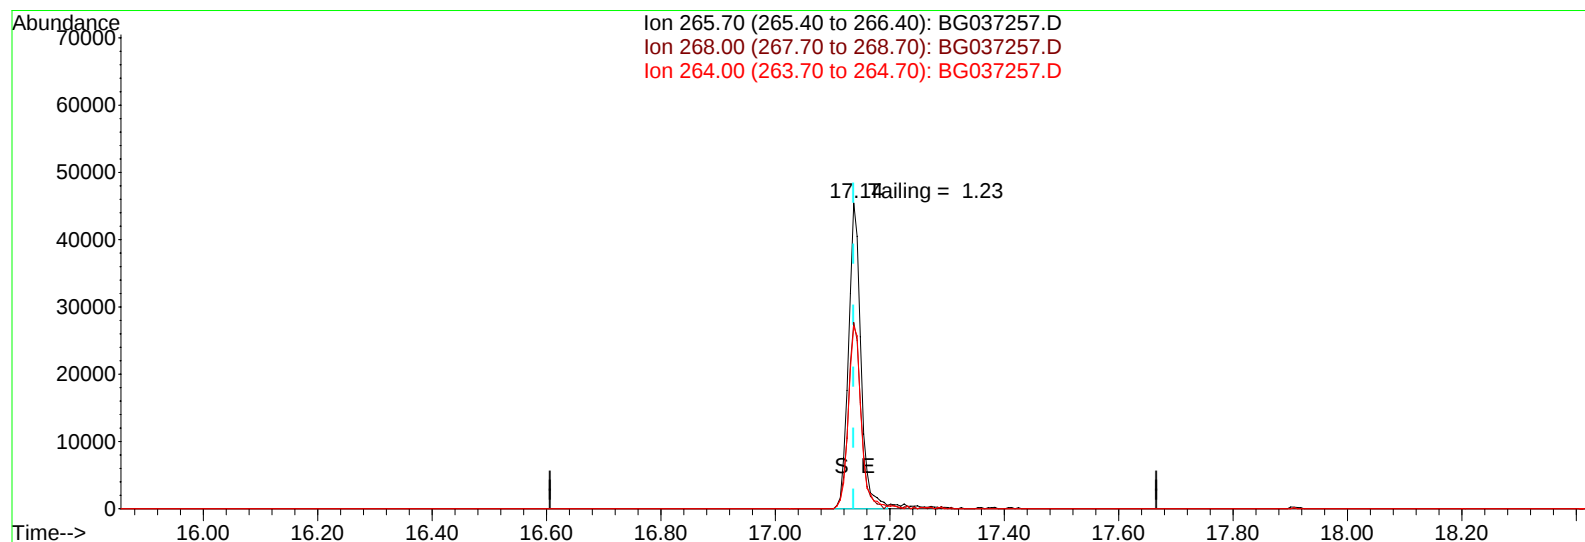

TIC: BG037257.D

(70) Pentachlorophenol (C)




17.137min (+0.001) 23976.29ng

response 69931

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.24
264.00	73.60	59.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\
Data File : BG037257.D
Acq On : 11 Oct 2018 14:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 17:03:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

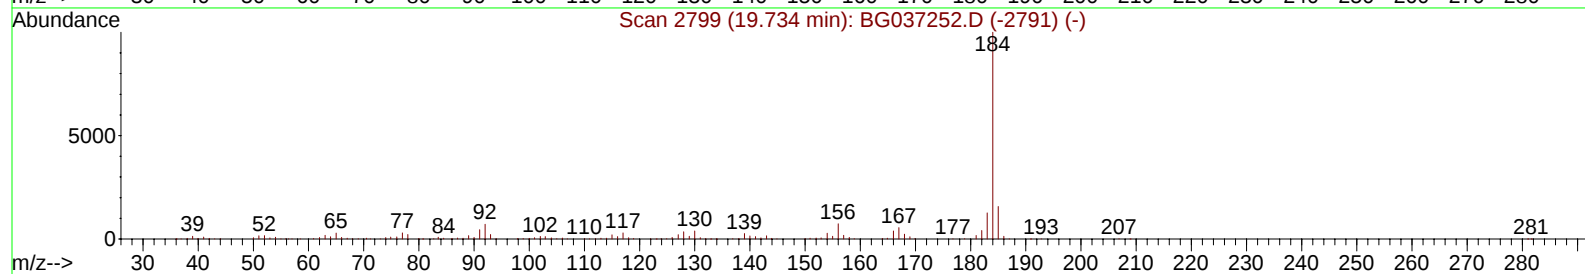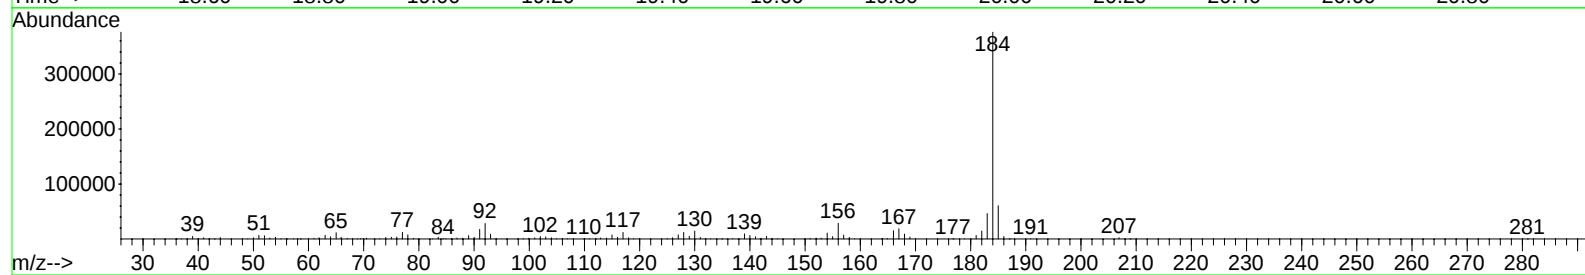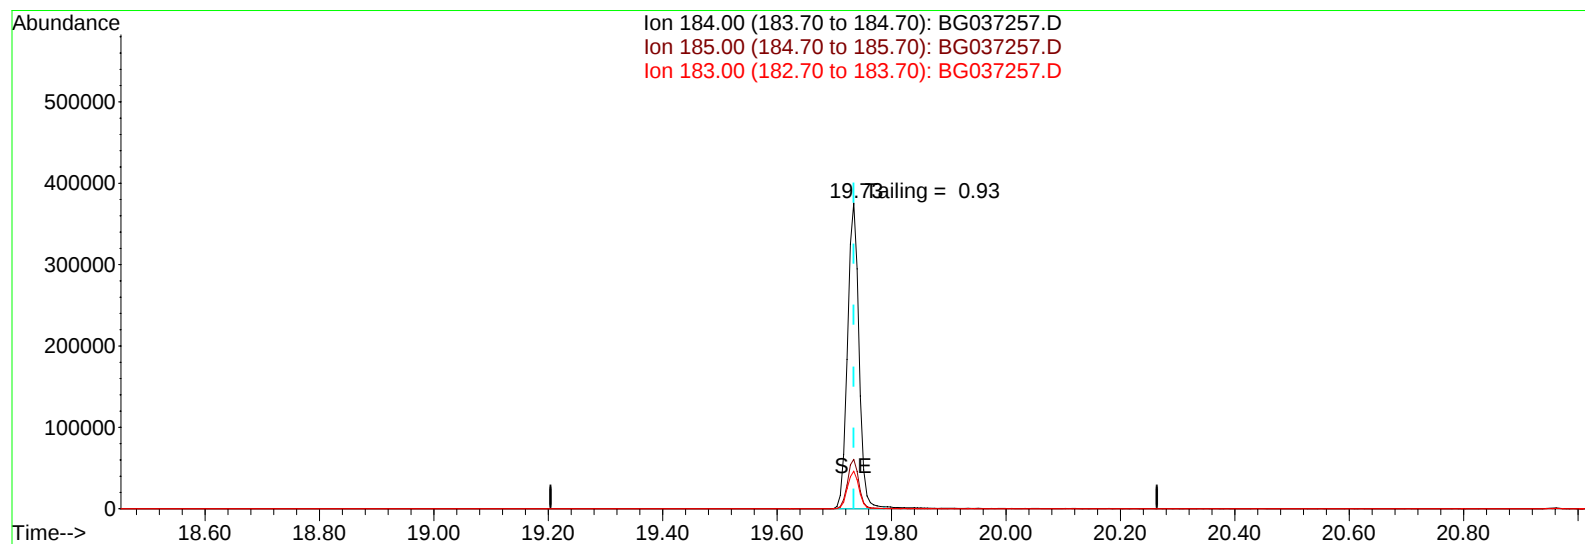

TIC: BG037257.D

(77) Benzidine

19.734min (-0.000) 0.00ng

response 531422

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.17
183.00	12.70	12.33
0.00	0.00	0.00