
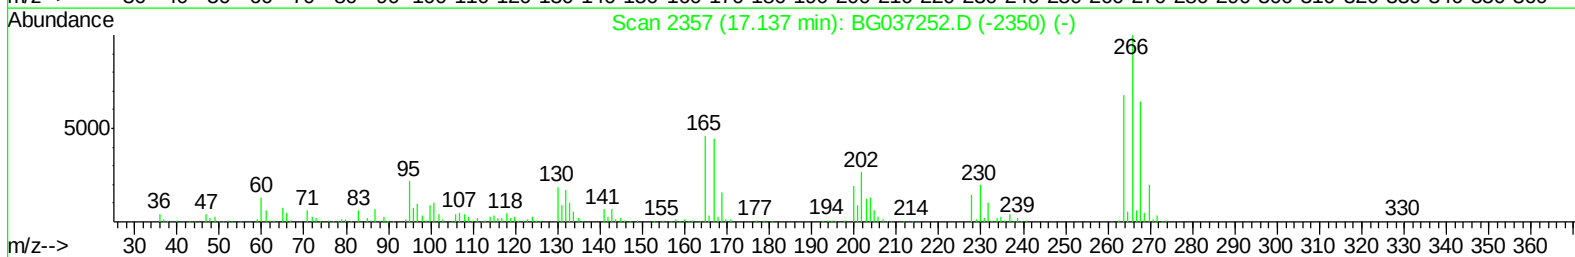
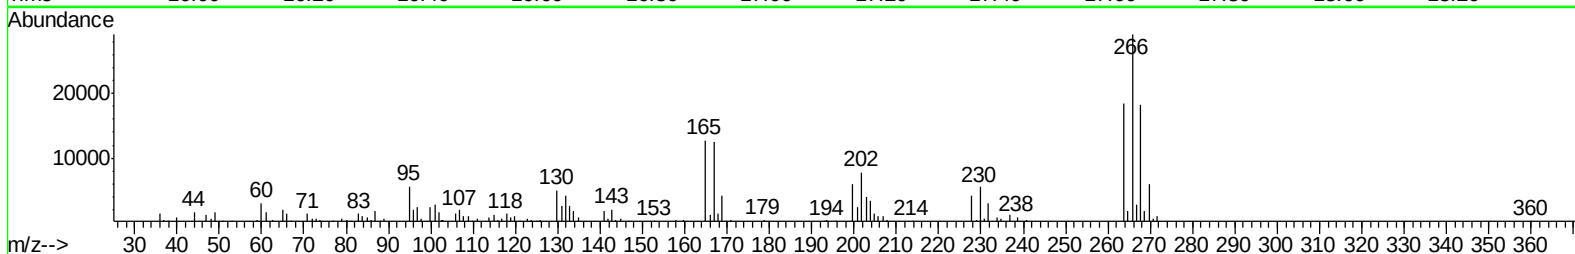


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101118\  
Data File : BG037275.D  
Acq On : 12 Oct 2018 3:49  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 09:05:44 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG101118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 11 13:59:58 2018  
Response via : Initial Calibration

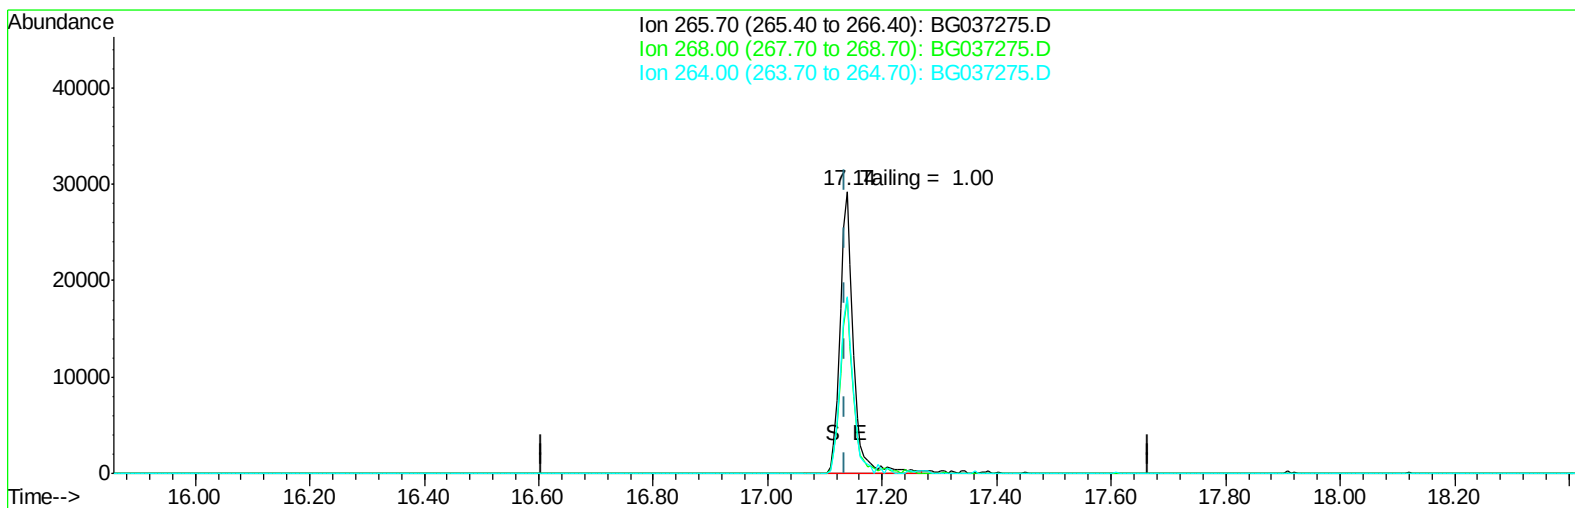

TIC: BG037275.D

(70) Pentachlorophenol (C)




17.139min (+0.003) 30434.16ng

response 46141

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 68.80 | 67.99 |
| 264.00 | 73.60 | 69.07 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101118\  
Data File : BG037275.D  
Acq On : 12 Oct 2018 3:49  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 09:05:44 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG101118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 11 13:59:58 2018  
Response via : Initial Calibration

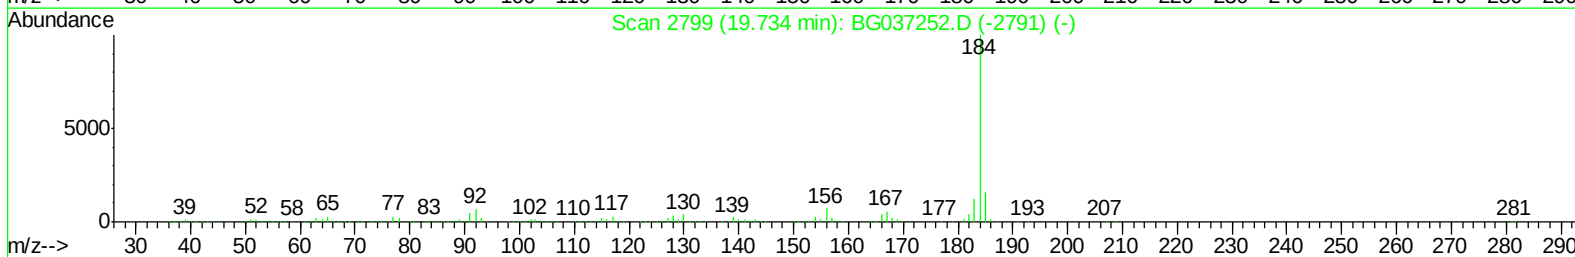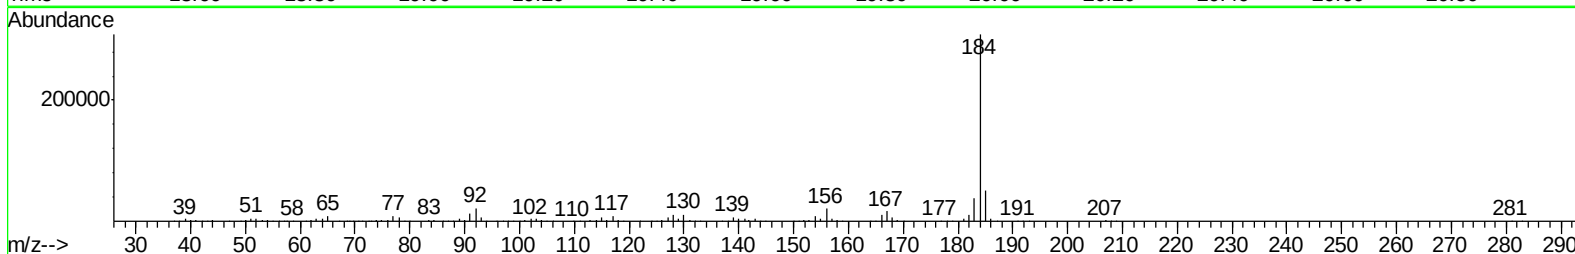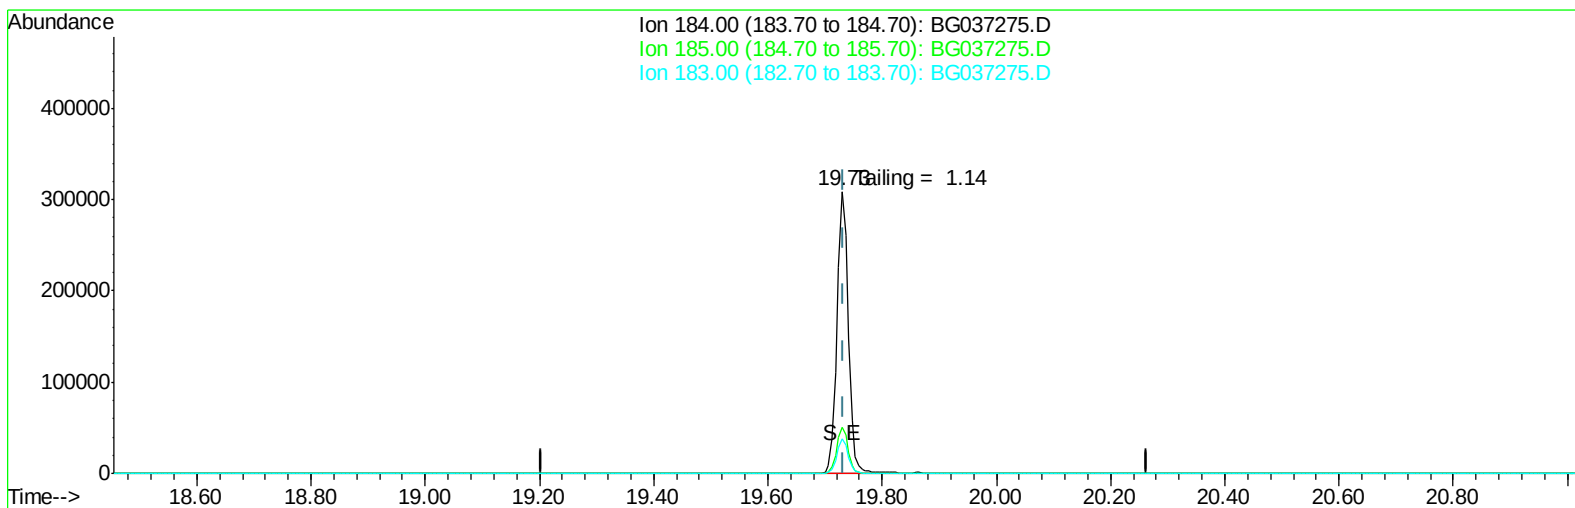

TIC: BG037275.D

(77) Benzidine

19.730min (-0.004) 0.00ng

response 427347

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 16.46 |
| 183.00 | 12.70 | 12.42 |
| 0.00   | 0.00  | 0.00  |