

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101118\
 Data File : BG037270.D
 Acq On : 11 Oct 2018 23:14
 Operator : JU/SJ
 Sample : J5373-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RT1499-3783-RT3026

Quant Time: Oct 12 07:15:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 11 13:59:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	54542	20.00	ng	0.00
21) Naphthalene-d8	10.94	136	232448	20.00	ng	0.00
39) Acenaphthene-d10	14.76	164	157350	20.00	ng	0.00
64) Phenanthrene-d10	17.50	188	411361	20.00	ng	0.00
76) Chrysene-d12	21.79	240	421266	20.00	ng	0.00
87) Perylene-d12	25.14	264	414007	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.66	112	351950	113.56	ng	0.00
7) Phenol-d6	7.26	99	467160	99.31	ng	0.00
23) Nitrobenzene-d5	9.30	82	297377	84.11	ng	0.00
42) 2,4,6-Tribromophenol	16.24	330	193353	125.30	ng	0.00
45) 2-Fluorobiphenyl	13.38	172	743635	70.97	ng	0.00
79) Terphenyl-d14	20.10	244	1430078	71.28	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101118\
Data File : BG037270.D
Acq On : 11 Oct 2018 23:14
Operator : JU/SJ
Sample : J5373-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RT1499-3783-RT3026

Quant Time: Oct 12 07:15:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 11 13:59:58 2018
Response via : Initial Calibration

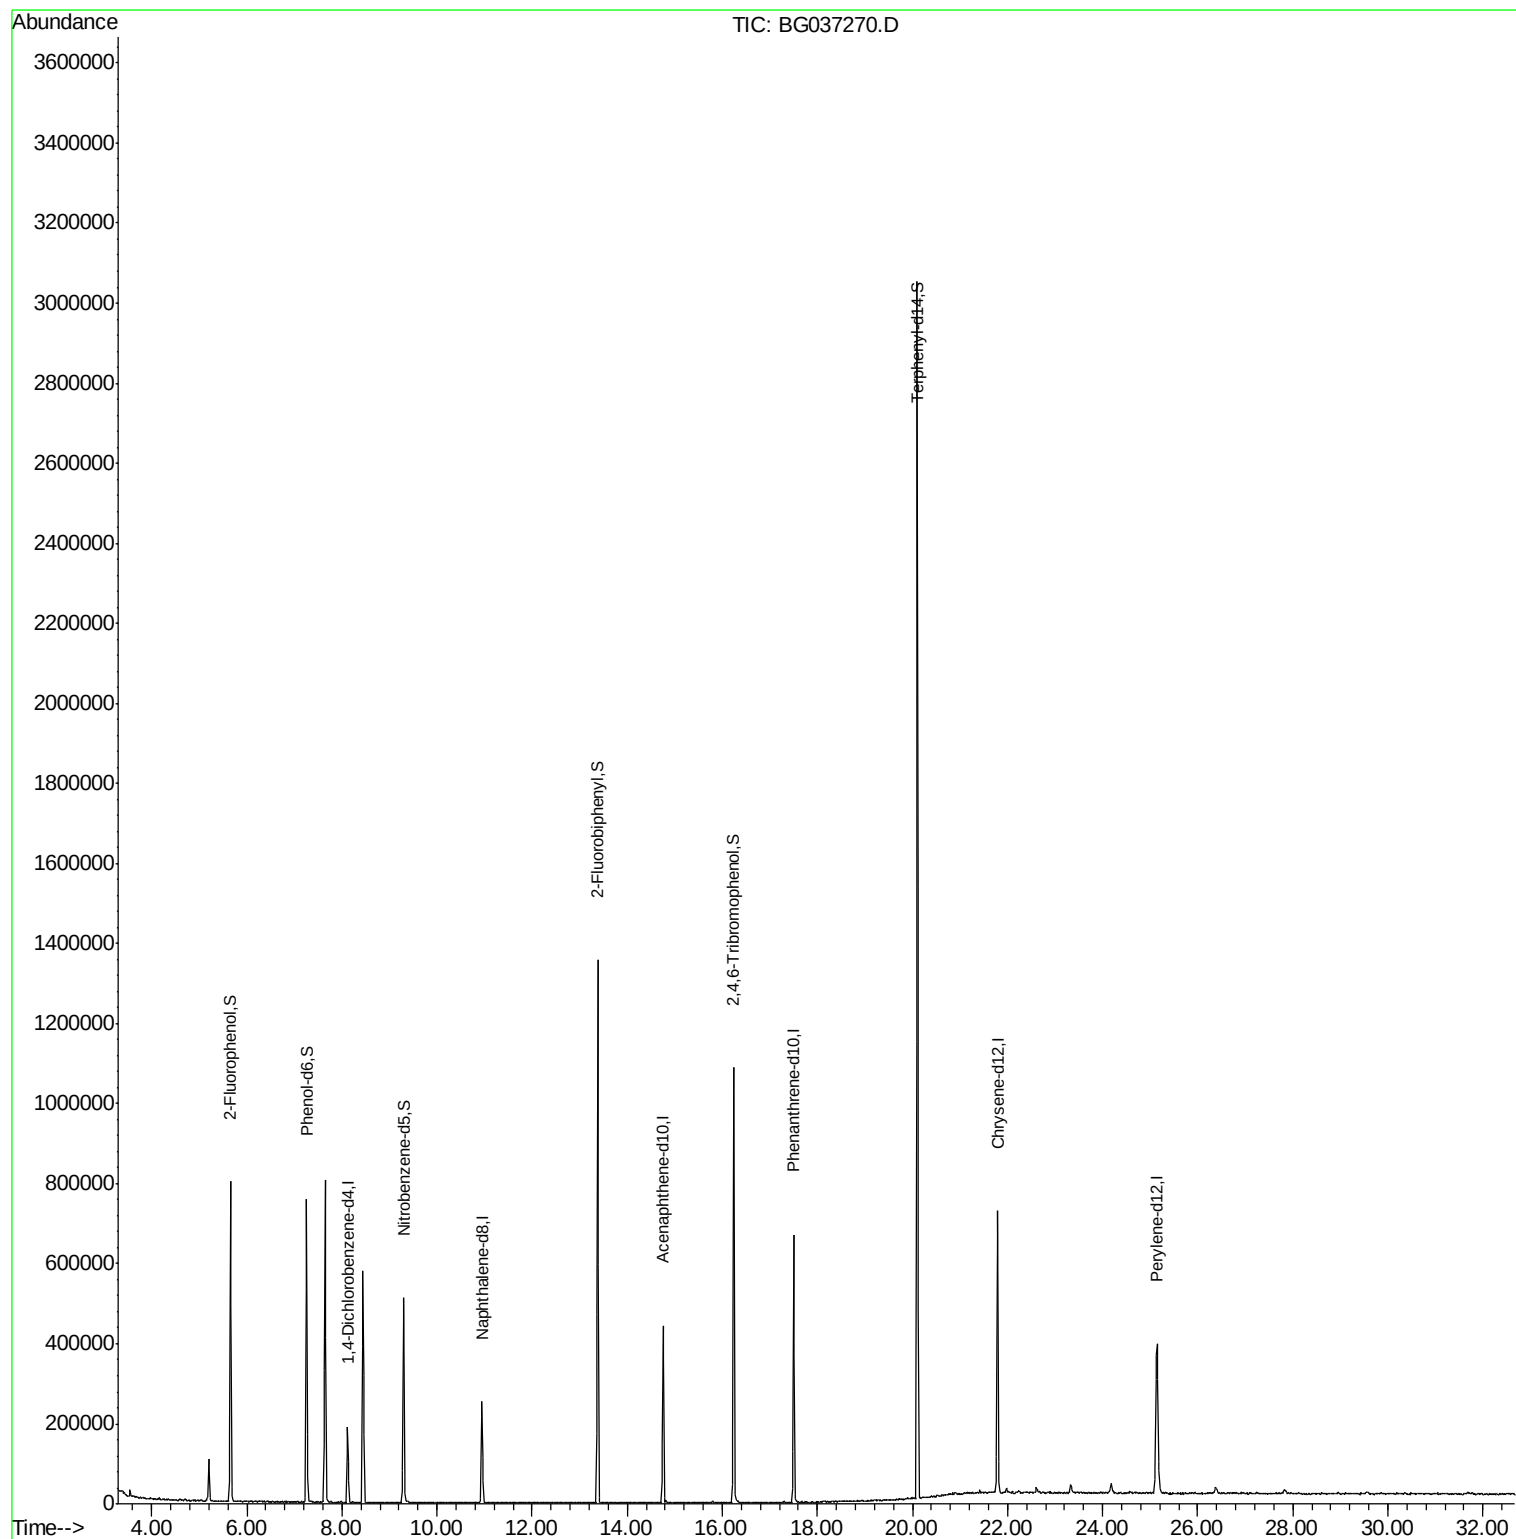




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.12 min Scan# 823
Delta R.T. -0.00 min
Lab File: BG037270.D
Acq: 11 Oct 2018 23:14

Instrument :
BNA_G
ClientSampleId :
RT1499-3783-RT3026

Tot Ion:152 Resp: 54542
Ion Ratio Lower Upper
152 100
150 157.0 126.0 189.0
115 59.5 45.5 68.3




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

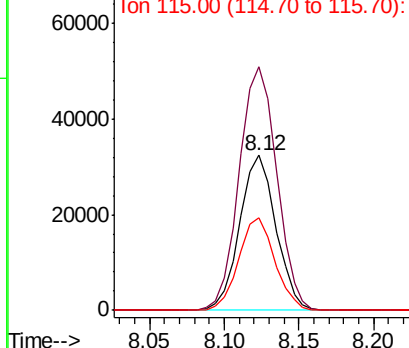



#5


2-Fluorophenol
Concen: 113.564 ng
RT: 5.66 min Scan# 403
Delta R.T. 0.01 min
Lab File: BG037270.D
Acq: 11 Oct 2018 23:14

Tgt Ion:112 Resp: 351950
Ion Ratio Lower Upper
112 100
64 71.3 53.1 79.7
63 34.4 27.3 40.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

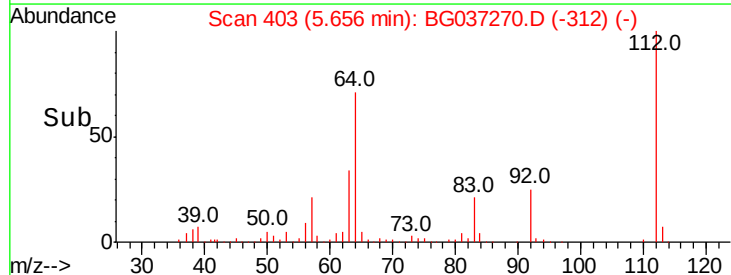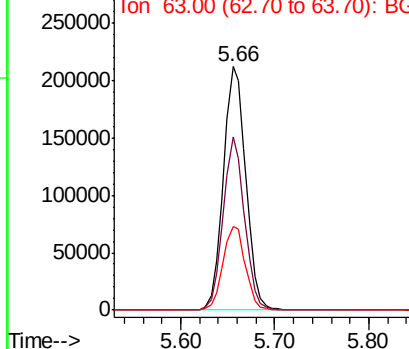



#7

Phenol-d6

Concen: 99.311 ng

RT: 7.26 min Scan# 676

Delta R.T. 0.01 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14

Instrument :

BNA_G

ClientSampleId :

RT1499-3783-RT3026


Tot Ion: 99 Resp: 467160

Ion Ratio Lower Upper




99 100

42 18.7 15.0 22.4

71 31.2 25.5 38.3

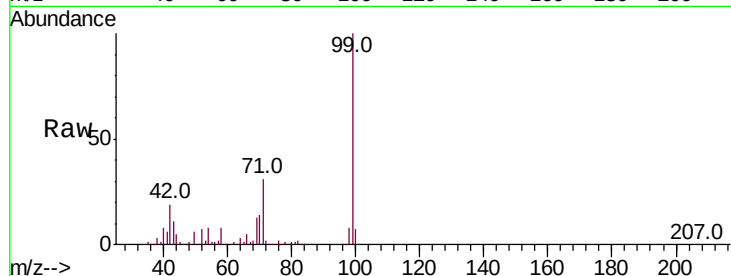

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

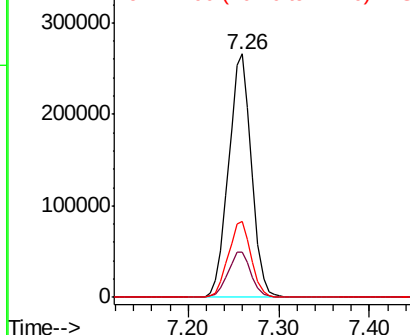

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.94 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14

Tgt Ion: 136 Resp: 232448


Ion Ratio Lower Upper

136 100



137 11.0 9.6 14.4


54 10.5 7.9 11.9

68 7.0 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

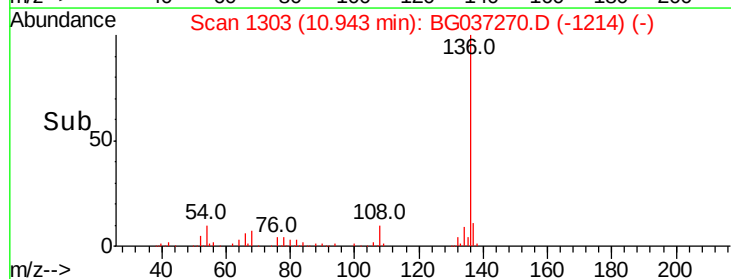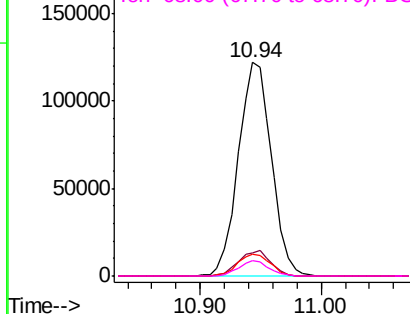


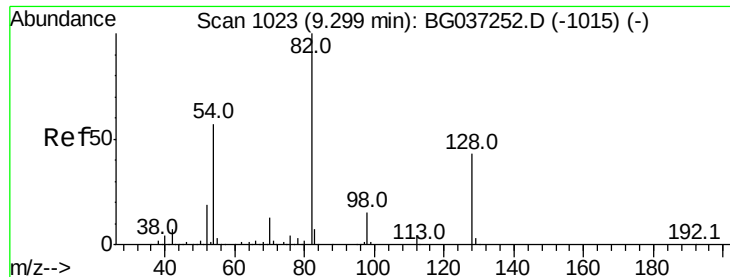




#23
 Nitrobenzene-d5
 Concen: 84.109 ng
 RT: 9.30 min Scan# 1023
 Delta R.T. -0.00 min
 Lab File: BG037270.D
 Acq: 11 Oct 2018 23:14

Instrument :
 BNA_G
 ClientSampleId :
 RT1499-3783-RT3026

Tot Ion	Ratio	Lower	Upper
82	100		
128	42.7	34.6	51.8
54	56.7	45.3	67.9

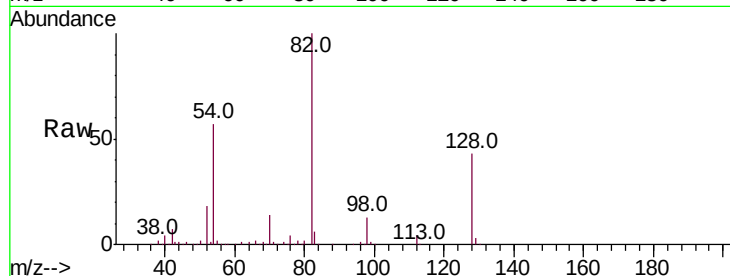


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

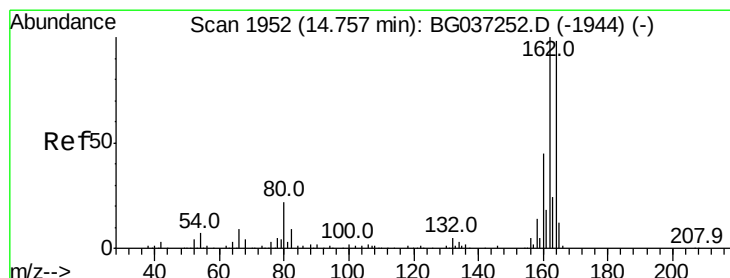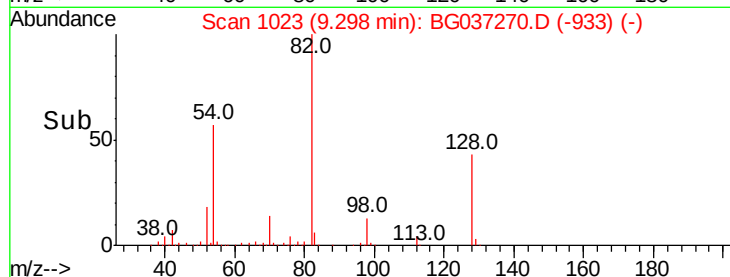
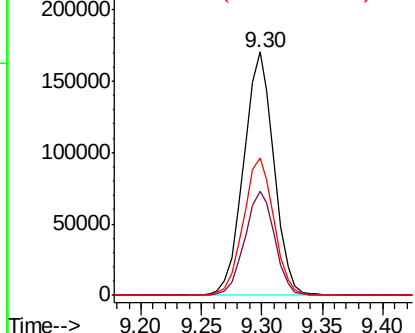



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.76 min Scan# 1952
 Delta R.T. -0.00 min
 Lab File: BG037270.D
 Acq: 11 Oct 2018 23:14

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.0	81.3	121.9
160	46.9	36.3	54.5

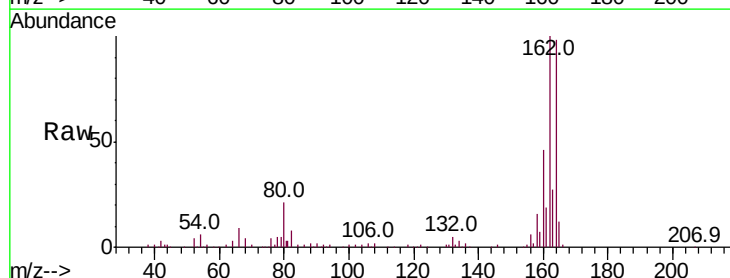

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

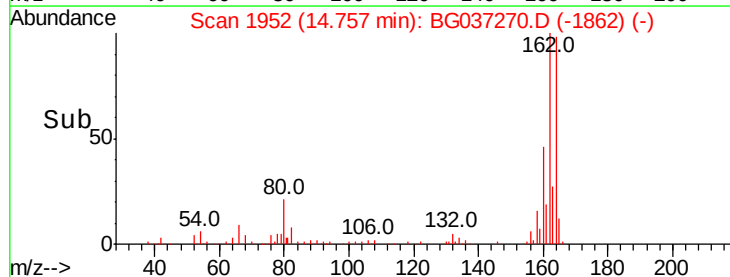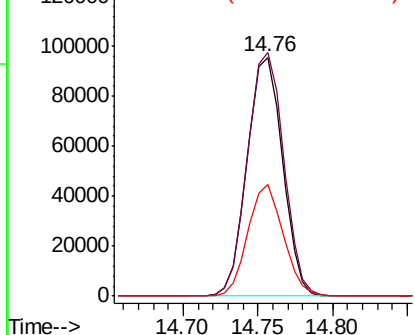







#42
 2,4,6-Tribromophenol
 Concen: 125.296 ng
 RT: 16.24 min Scan# 2205
 Delta R.T. -0.00 min
 Lab File: BG037270.D
 Acq: 11 Oct 2018 23:14

Instrument :
 BNA_G
 ClientSampleId :
 RT1499-3783-RT3026

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	78.4	117.6
141	40.6	32.2	48.2

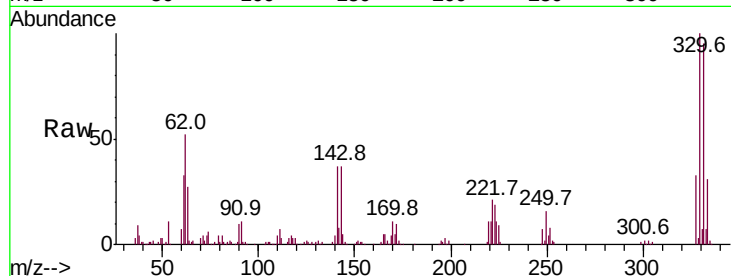


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


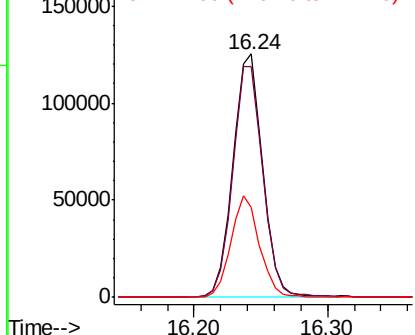



#45
 2-Fluorobiphenyl
 Concen: 70.973 ng
 RT: 13.38 min Scan# 1718
 Delta R.T. -0.00 min
 Lab File: BG037270.D
 Acq: 11 Oct 2018 23:14

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.4	31.0	46.4
170	24.3	20.2	30.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

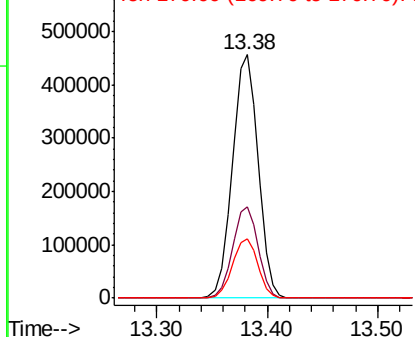



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.50 min Scan# 2419

Delta R.T. -0.01 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14

Instrument :

BNA_G

ClientSampleId :

RT1499-3783-RT3026



Tot Ion:188 Resp: 411361

Ion Ratio Lower Upper

188 100

94 9.4 7.2 10.8



80 9.9 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

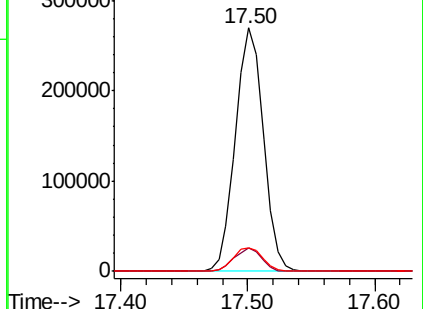

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.79 min Scan# 3149

Delta R.T. -0.01 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14



Tgt Ion:240 Resp: 421266

Ion Ratio Lower Upper

240 100

120 10.9 8.1 12.1


236 26.5 21.4 32.0




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

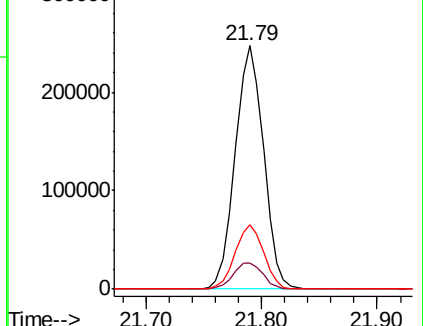

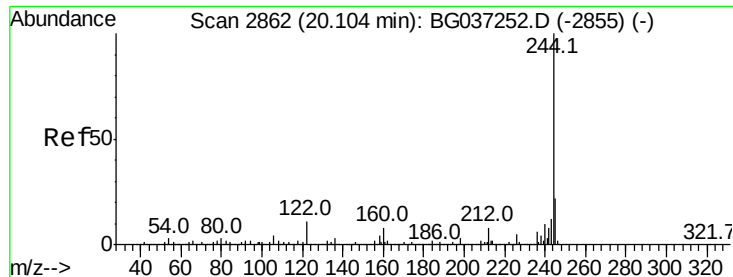

#79

Terphenyl-d14

Concen: 71.281 ng

RT: 20.10 min Scan# 2862

Delta R.T. -0.00 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14

Instrument :

BNA_G

ClientSampleId :

RT1499-3783-RT3026


Tot Ion:244 Resp: 1430078

Ion Ratio Lower Upper

244 100

212 8.9 6.5 9.7




122 12.0 9.0 13.4

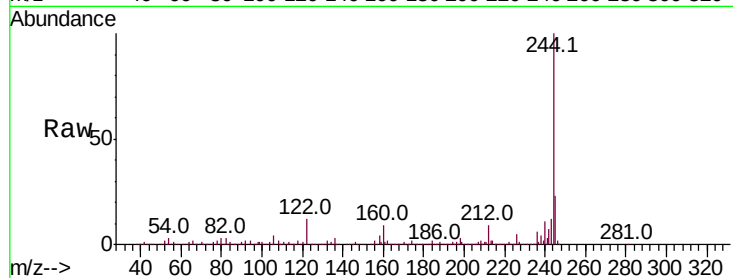

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

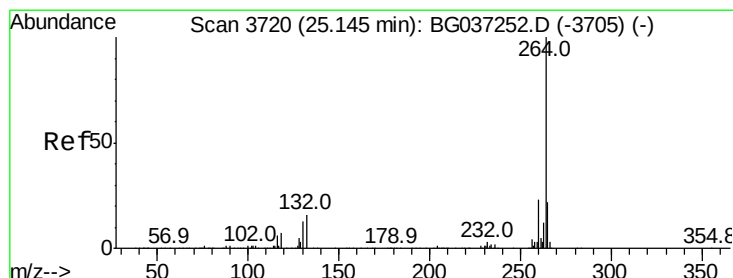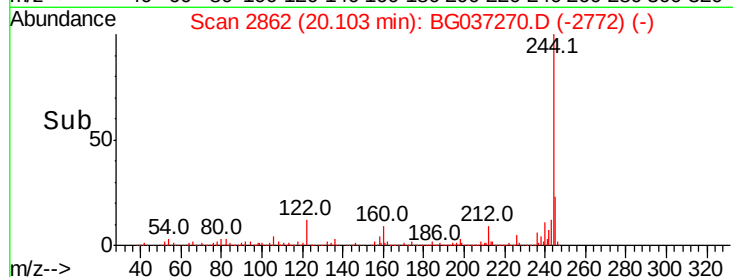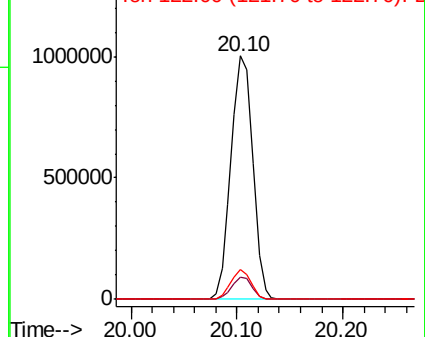

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.14 min Scan# 3720

Delta R.T. -0.00 min

Lab File: BG037270.D

Acq: 11 Oct 2018 23:14


Tgt Ion:264 Resp: 414007

Ion Ratio Lower Upper

264 100

260 24.1 18.2 27.4

265 22.5 17.9 26.9

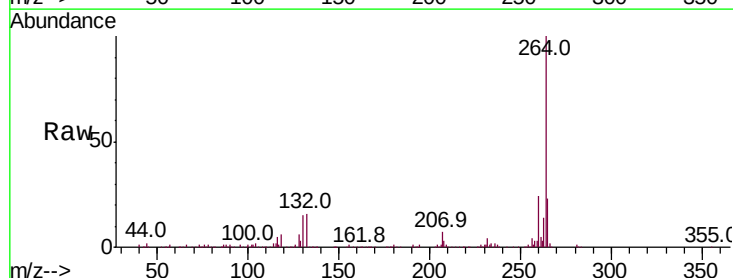

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

