


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\  
 Data File : BG037248.D  
 Acq On : 11 Oct 2018 8:28  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG101118.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Oct 11 13:59:58 2018

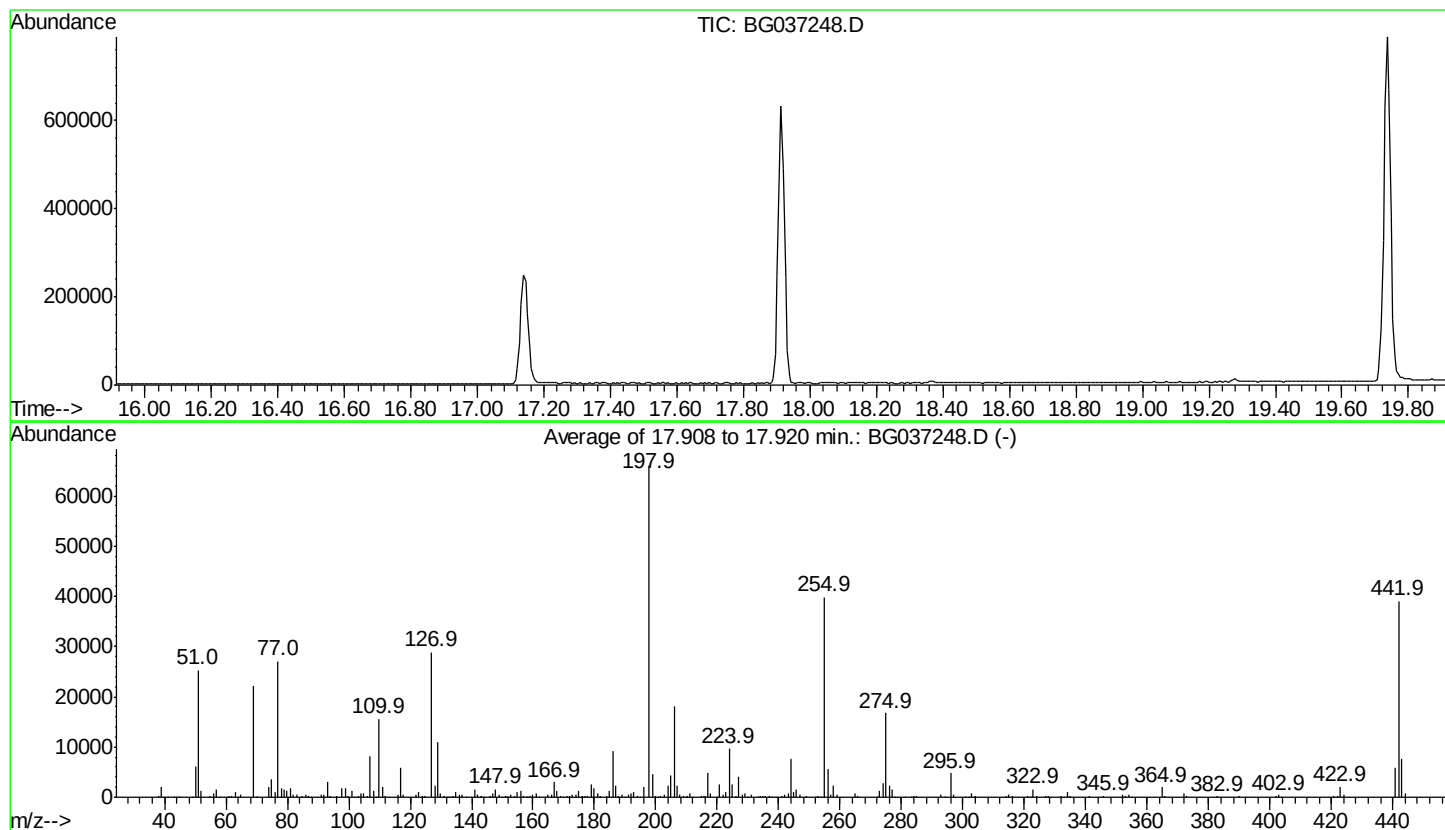

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 38.3      | 25317   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 33.5      | 22120   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 59      | PASS             |
| 127         | 198          | 10           | 80           | 43.8      | 28904   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 66021   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 4468    | PASS             |
| 275         | 198          | 10           | 60           | 25.3      | 16727   | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 1997    | PASS             |
| 441         | 198          | 0.01         | 100          | 8.9       | 5854    | PASS             |
| 442         | 198          | 50           | 100          | 59.2      | 39074   | PASS             |
| 443         | 442          | 15           | 24           | 19.9      | 7775    | PASS             |