


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG101118\
 Data File : BG037257.D
 Acq On : 11 Oct 2018 14:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 11 13:59:58 2018

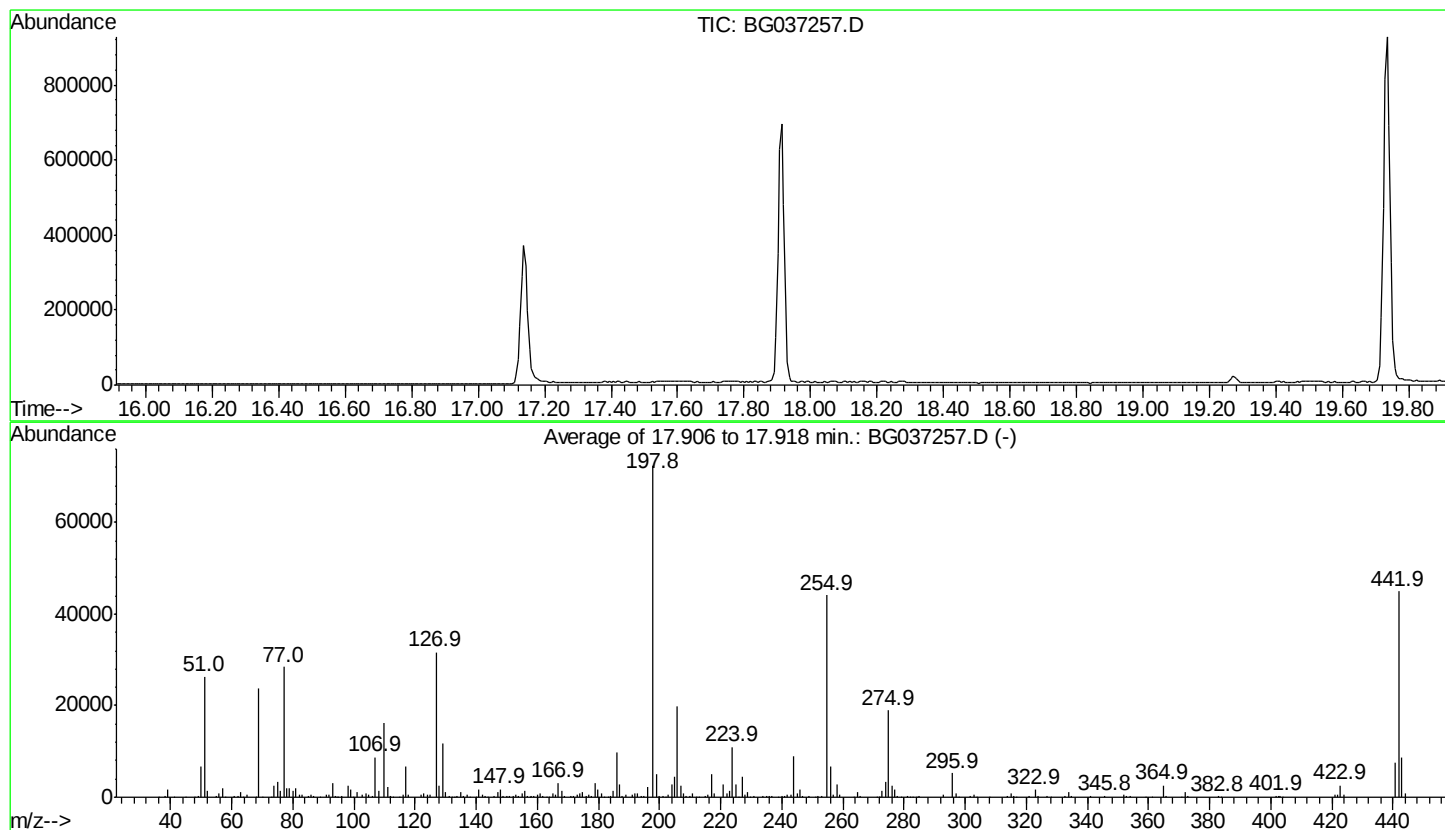

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	26406	PASS
68	69	0.00	2	0.5	122	PASS
69	198	0.00	100	32.7	23701	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	43.7	31629	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72426	PASS
199	198	5	9	7.0	5100	PASS
275	198	10	60	26.2	18984	PASS
365	198	1	100	3.5	2545	PASS
441	198	0.01	100	10.4	7547	PASS
442	198	50	100	62.0	44896	PASS
443	442	15	24	19.5	8777	PASS