

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050536.D
 Acq On : 11 Oct 2021 14:23
 Operator : CG/JU
 Sample : M4144-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IDW-LIQ-DRUM-2-100721

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050536.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.787	46	51	61	rVB	32111	54235	1.81%	0.212%
2	4.263	124	132	147	rBV5	25621	87019	2.90%	0.340%
3	4.392	149	154	160	rVB2	21647	39716	1.33%	0.155%
4	5.320	306	312	319	rBV	95006	163396	5.45%	0.638%
5	5.620	357	363	367	rBV	20394	34811	1.16%	0.136%
6	5.679	367	373	376	rVV	35718	71874	2.40%	0.281%
7	5.714	376	379	385	rVB	29514	48051	1.60%	0.188%
8	5.796	386	393	403	rVB	621219	1046704	34.93%	4.085%
9	6.307	472	480	493	rVB2	21451	49239	1.64%	0.192%
10	7.259	626	642	647	rBV	84685	249311	8.32%	0.973%
11	7.335	649	655	659	rVV2	24556	48859	1.63%	0.191%
12	7.400	659	666	675	rVV	586551	1073314	35.81%	4.189%
13	7.488	675	681	686	rVV4	23768	48209	1.61%	0.188%
14	7.776	725	730	734	rBV	20752	32052	1.07%	0.125%
15	7.829	734	739	748	rVV	56625	103029	3.44%	0.402%
16	8.017	766	771	777	rVB	36972	60406	2.02%	0.236%
17	8.264	802	813	818	rBV	198580	372332	12.42%	1.453%
18	8.305	818	820	826	rVV	28156	34401	1.15%	0.134%
19	8.834	897	910	919	rBV2	81775	216088	7.21%	0.843%
20	9.098	949	955	960	rVB5	18422	31690	1.06%	0.124%
21	9.433	1004	1012	1021	rBV	452008	870256	29.04%	3.396%
22	9.521	1021	1027	1032	rVV2	26255	52075	1.74%	0.203%
23	10.314	1155	1162	1166	rBV2	23931	49794	1.66%	0.194%
24	10.391	1166	1175	1181	rVB2	124819	288781	9.64%	1.127%
25	10.831	1242	1250	1261	rBV	722439	1268806	42.34%	4.952%
26	11.084	1284	1293	1302	rBV	263372	505002	16.85%	1.971%
27	11.848	1415	1423	1432	rBV2	76462	154163	5.14%	0.602%
28	12.371	1508	1512	1518	rVB3	19720	30552	1.02%	0.119%
29	13.135	1637	1642	1647	rBV2	41886	68055	2.27%	0.266%
30	13.505	1694	1705	1711	rBV	1055258	1686523	56.28%	6.582%
31	13.752	1741	1747	1749	rBV	59006	97012	3.24%	0.379%
32	13.775	1749	1751	1754	rVV	53325	77608	2.59%	0.303%
33	13.816	1754	1758	1765	rVB	223359	335436	11.19%	1.309%
34	14.398	1851	1857	1864	rBV4	19853	34295	1.14%	0.134%
35	14.492	1864	1873	1888	rBV	769024	1324601	44.20%	5.170%
36	14.821	1924	1929	1933	rBV2	51657	78015	2.60%	0.304%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050536.D
 Acq On : 11 Oct 2021 14:23
 Operator : CG/JU
 Sample : M4144-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IDW-LIQ-DRUM-2-100721

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.880	1933	1939	1948	rVB	399745	662575	22.11%	2.586%
38	15.273	1995	2006	2011	rBV2	387151	662810	22.12%	2.587%
39	15.444	2030	2035	2040	rBV	27443	42984	1.43%	0.168%
40	15.596	2057	2061	2065	rBV	30028	43368	1.45%	0.169%
41	15.761	2083	2089	2092	rBV2	19542	35784	1.19%	0.140%
42	15.808	2092	2097	2099	rVV4	29136	55300	1.85%	0.216%
43	15.843	2099	2103	2108	rVB2	53559	84116	2.81%	0.328%
44	16.043	2133	2137	2142	rVB2	44887	67761	2.26%	0.264%
45	16.143	2149	2154	2159	rBV	41374	58199	1.94%	0.227%
46	16.307	2174	2182	2185	rBV6	21238	45391	1.51%	0.177%
47	16.384	2185	2195	2210	rVV3	1208232	2996922	100.00%	11.696%
48	16.736	2251	2255	2261	rVB6	19627	34162	1.14%	0.133%
49	16.830	2267	2271	2275	rBV	27205	36320	1.21%	0.142%
50	16.871	2275	2278	2282	rVB	26913	35370	1.18%	0.138%
51	16.983	2293	2297	2306	rVB2	68292	112384	3.75%	0.439%
52	17.077	2308	2313	2320	rVB10	20661	39830	1.33%	0.155%
53	17.183	2326	2331	2335	rBV	32428	52079	1.74%	0.203%
54	17.623	2394	2406	2413	rBV	488608	818760	27.32%	3.195%
55	17.688	2414	2417	2424	rVB	26773	41241	1.38%	0.161%
56	17.858	2443	2446	2451	rBV	26851	35956	1.20%	0.140%
57	17.911	2451	2455	2460	rVB3	24166	37501	1.25%	0.146%
58	17.970	2460	2465	2479	rBV	261542	418202	13.95%	1.632%
59	18.146	2490	2495	2502	rVB	48307	78973	2.64%	0.308%
60	18.258	2510	2514	2518	rBV	84453	112031	3.74%	0.437%
61	18.323	2522	2525	2533	rVB2	42226	62329	2.08%	0.243%
62	18.411	2536	2540	2546	rVB2	38915	48331	1.61%	0.189%
63	18.487	2547	2553	2563	rBV	572659	839502	28.01%	3.276%
64	18.587	2567	2570	2574	rVB	46934	62023	2.07%	0.242%
65	18.857	2612	2616	2625	rBV2	49867	103432	3.45%	0.404%
66	19.333	2693	2697	2702	rBV7	24515	39383	1.31%	0.154%
67	19.392	2703	2707	2708	rVV4	40000	52535	1.75%	0.205%
68	19.415	2708	2711	2720	rVB	146597	188937	6.30%	0.737%
69	19.744	2763	2767	2782	rVB	252826	392997	13.11%	1.534%
70	19.962	2802	2804	2807	rVV	31053	30119	1.00%	0.118%
71	20.003	2807	2811	2818	rVB3	75939	105293	3.51%	0.411%
72	20.209	2838	2846	2852	rBV	1548873	2162239	72.15%	8.439%
73	20.467	2886	2890	2891	rBV4	49146	58534	1.95%	0.228%
74	20.491	2891	2894	2899	rVB	96741	119720	3.99%	0.467%
75	20.831	2949	2952	2954	rBV2	37295	41304	1.38%	0.161%
76	20.861	2954	2957	2966	rVB7	54519	104676	3.49%	0.409%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050536.D
 Acq On : 11 Oct 2021 14:23
 Operator : CG/JU
 Sample : M4144-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 IDW-LIQ-DRUM-2-100721

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	20.996	2975	2980	2984	rBV	158045	202532	6.76%	0.790%
78	21.031	2984	2986	2989	rVB2	28970	30867	1.03%	0.120%
79	21.519	3065	3069	3080	rVB	325387	555825	18.55%	2.169%
80	21.619	3083	3086	3094	rVB	45832	64362	2.15%	0.251%
81	21.924	3132	3138	3146	rVB	437804	758213	25.30%	2.959%
82	22.095	3163	3167	3174	rVB	158992	236223	7.88%	0.922%
83	22.741	3271	3277	3291	rVB	141389	282286	9.42%	1.102%
84	23.140	3339	3345	3352	rVB	189106	337745	11.27%	1.318%
85	23.470	3396	3401	3409	rVB	113071	228420	7.62%	0.891%
86	24.333	3542	3548	3555	rVB2	83977	186005	6.21%	0.726%
87	25.338	3709	3719	3731	rVB3	315051	935544	31.22%	3.651%




Sum of corrected areas: 25623105

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050536.D
Acq On : 11 Oct 2021 14:23
Operator : CG/JU
Sample : M4144-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IDW-LIQ-DRUM-2-100721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

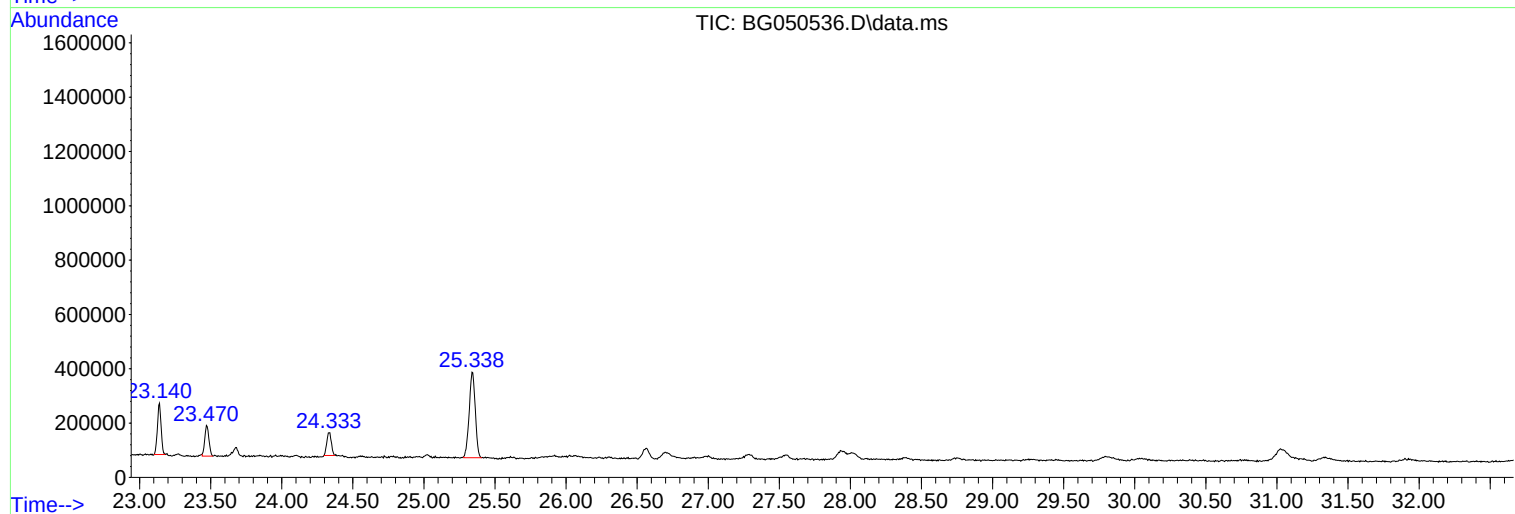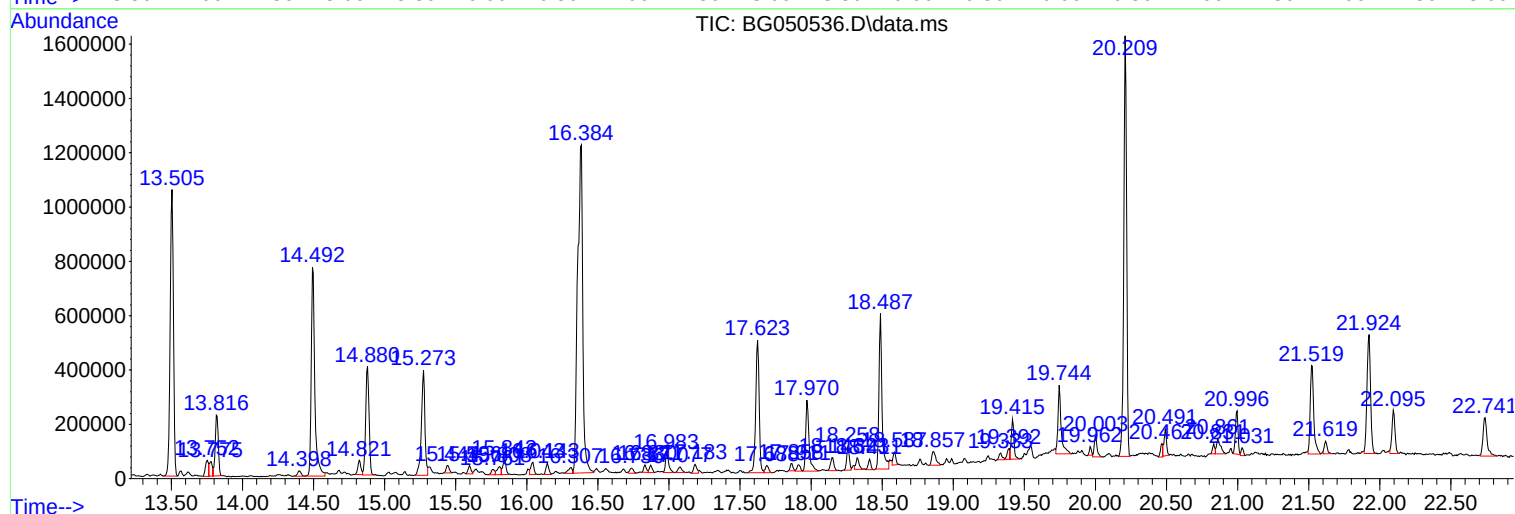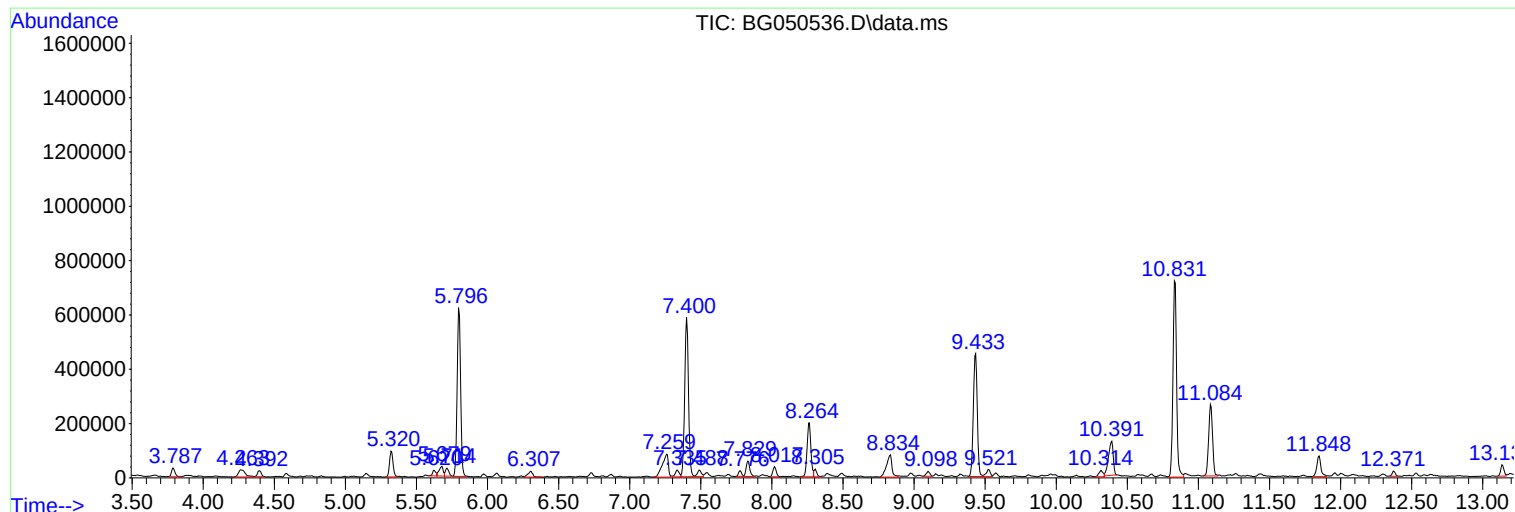

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050536.D
Acq On : 11 Oct 2021 14:23
Operator : CG/JU
Sample : M4144-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IDW-LIQ-DRUM-2-100721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050536.D
Acq On : 11 Oct 2021 14:23
Operator : CG/JU
Sample : M4144-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
IDW-LIQ-DRUM-2-100721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
