

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050542.D
 Acq On : 11 Oct 2021 19:29
 Operator : CG/JU
 Sample : M4112-02 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 1-ENTRANCE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.716	203	209	220	rVB	39492	62108	6.06%	1.064%
2	5.327	306	313	322	rVB	38011	63896	6.23%	1.095%
3	5.791	387	392	400	rVB2	32059	55360	5.40%	0.949%
4	7.395	657	665	675	rBV	51890	97024	9.47%	1.663%
5	8.259	805	812	820	rBV	256310	440399	42.97%	7.548%
6	9.428	1004	1011	1019	rBV	41626	76805	7.49%	1.316%
7	10.832	1245	1250	1255	rBV4	5606	11401	1.11%	0.195%
8	11.085	1282	1293	1302	rBV	358927	668844	65.26%	11.463%
9	13.500	1697	1704	1713	rBV	101226	157256	15.34%	2.695%
10	14.875	1931	1938	1950	rVB	550020	877289	85.60%	15.036%
11	16.361	2186	2191	2197	rBV5	11878	18606	1.82%	0.319%
12	17.618	2398	2405	2417	rBV	622990	996361	97.21%	17.077%
13	18.259	2510	2514	2517	rBV5	7762	11029	1.08%	0.189%
14	18.764	2596	2600	2603	rBV5	10320	11843	1.16%	0.203%
15	19.657	2745	2752	2756	rBV2	14607	27884	2.72%	0.478%
16	19.886	2787	2791	2795	rBV5	11508	16571	1.62%	0.284%
17	20.016	2811	2813	2817	rVB2	10225	11473	1.12%	0.197%
18	20.204	2840	2845	2851	rBV	156529	203550	19.86%	3.489%
19	20.926	2965	2968	2969	rBV3	12313	13412	1.31%	0.230%
20	21.614	3083	3085	3089	rBV2	11425	15494	1.51%	0.266%
21	21.919	3130	3137	3149	rVB	544584	973173	94.95%	16.679%
22	25.333	3708	3718	3732	rVB2	330092	1024911	100.00%	17.566%




Sum of corrected areas: 5834689

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050542.D
Acq On : 11 Oct 2021 19:29
Operator : CG/JU
Sample : M4112-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
1-ENTRANCE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

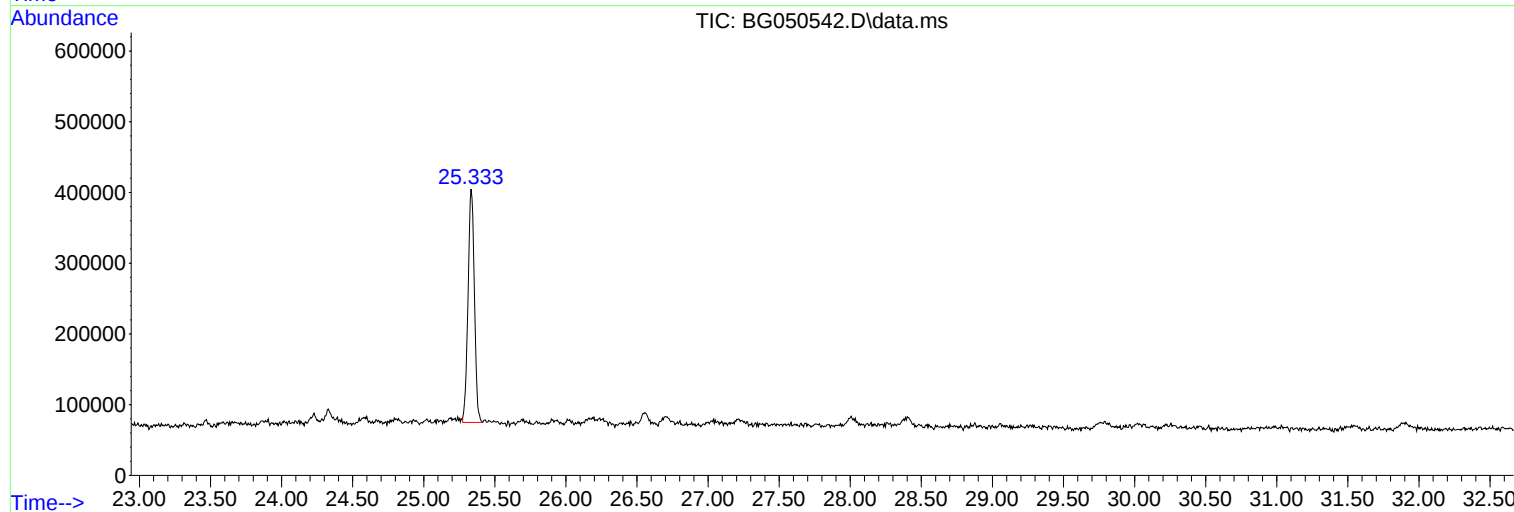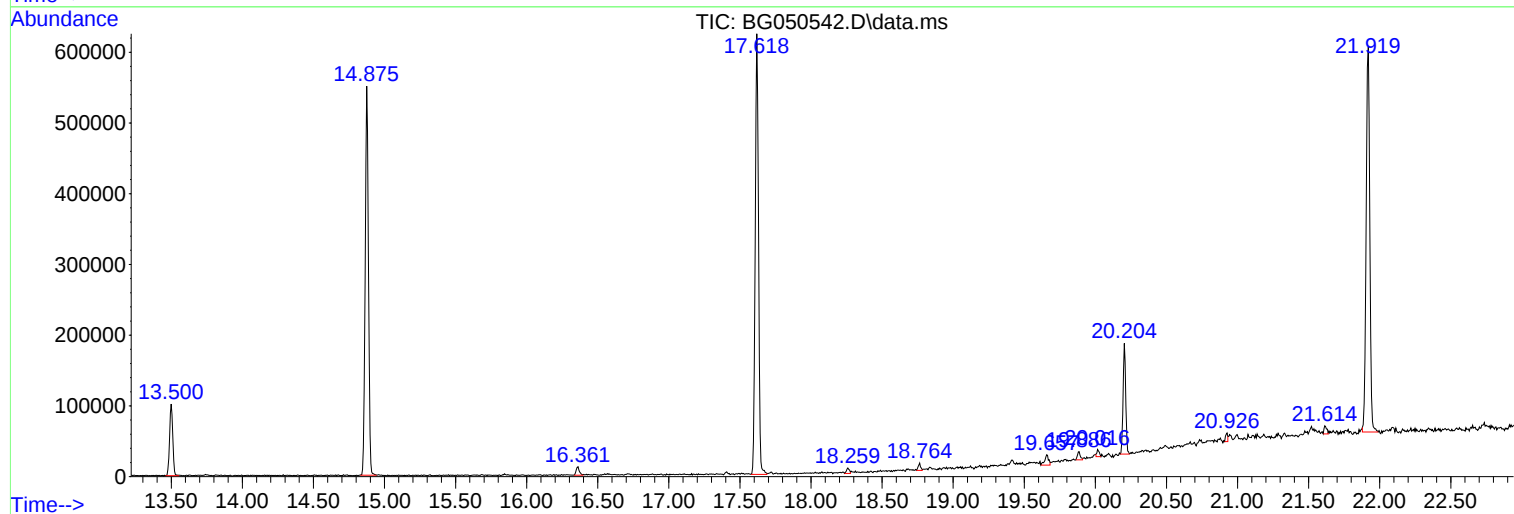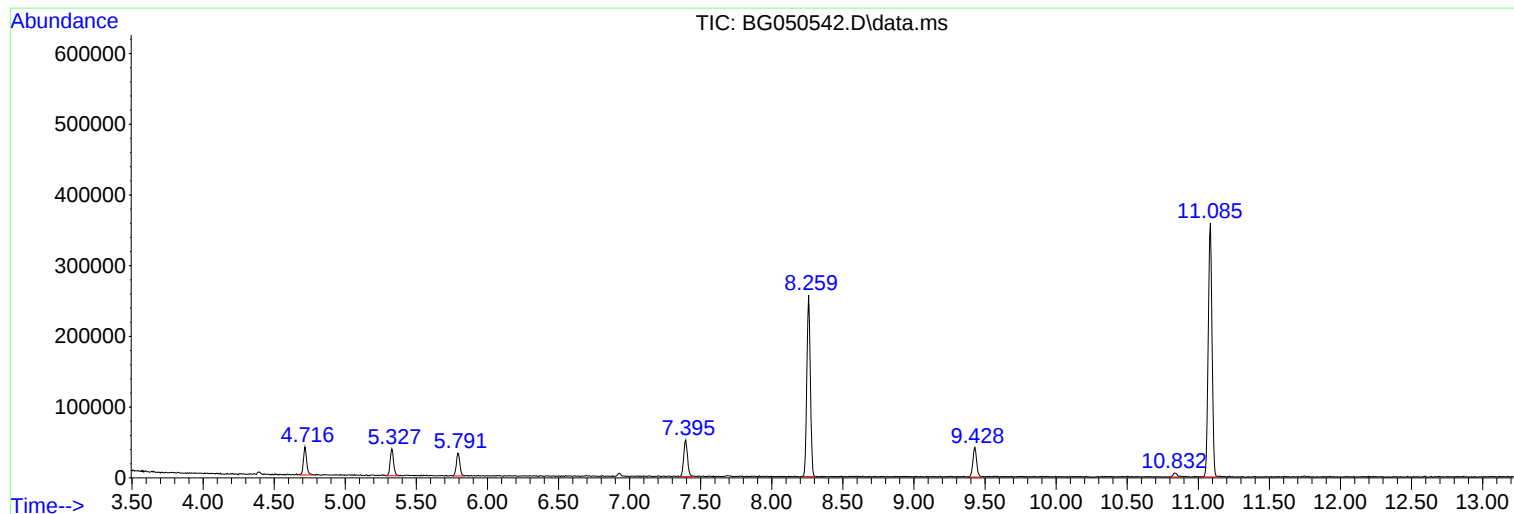

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050542.D
Acq On : 11 Oct 2021 19:29
Operator : CG/JU
Sample : M4112-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
1-ENTRANCE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050542.D
Acq On : 11 Oct 2021 19:29
Operator : CG/JU
Sample : M4112-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
1-ENTRANCE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
