


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050530.D
 Acq On : 11 Oct 2021 8:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

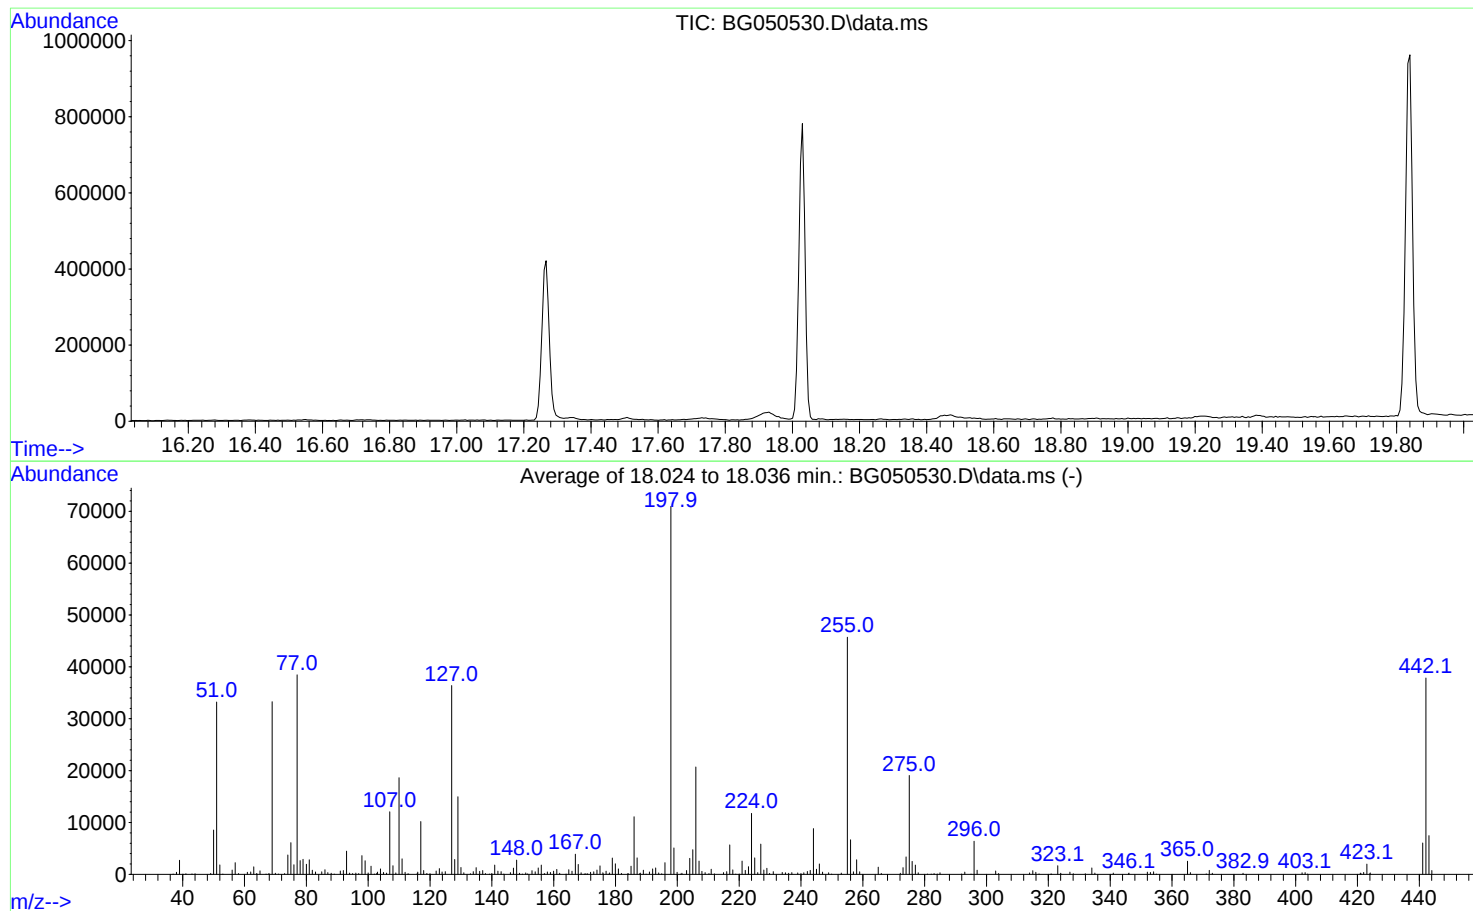




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	33227	PASS
68	69	0.00	2	0.6	191	PASS
69	198	0.00	100	46.9	33277	PASS
70	69	0.00	2	0.7	227	PASS
127	198	10	80	51.3	36392	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70912	PASS
199	198	5	9	7.2	5077	PASS
275	198	10	60	26.9	19070	PASS
365	198	1	100	3.6	2522	PASS
441	198	0.01	100	8.5	6038	PASS
442	442	50	100	100.0	37837	PASS
443	442	15	24	19.7	7463	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
 Data File : BG050530.D
 Acq On : 11 Oct 2021 8:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 11 11:11:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

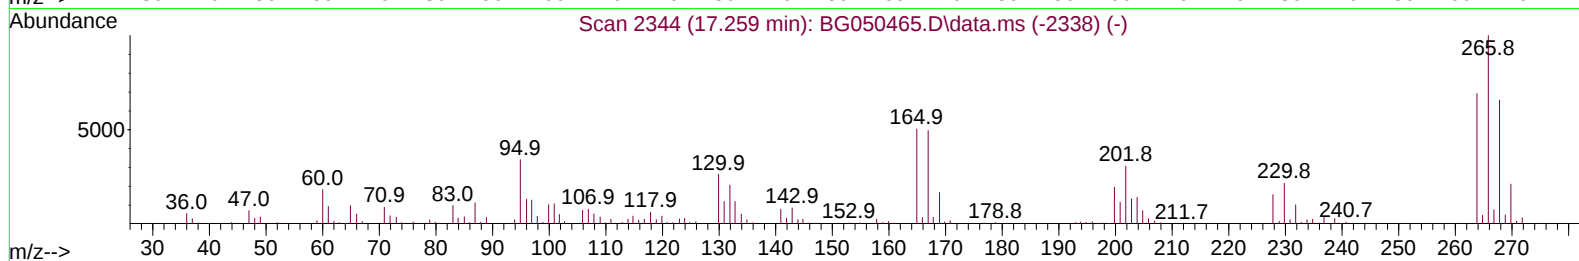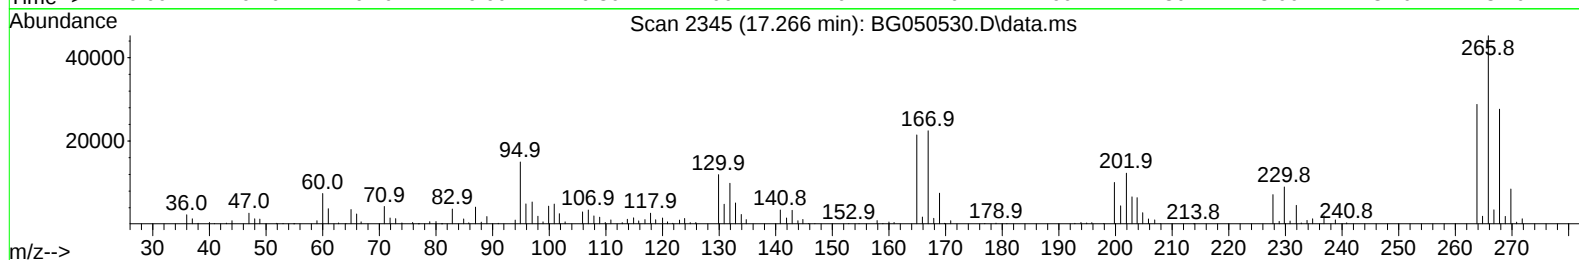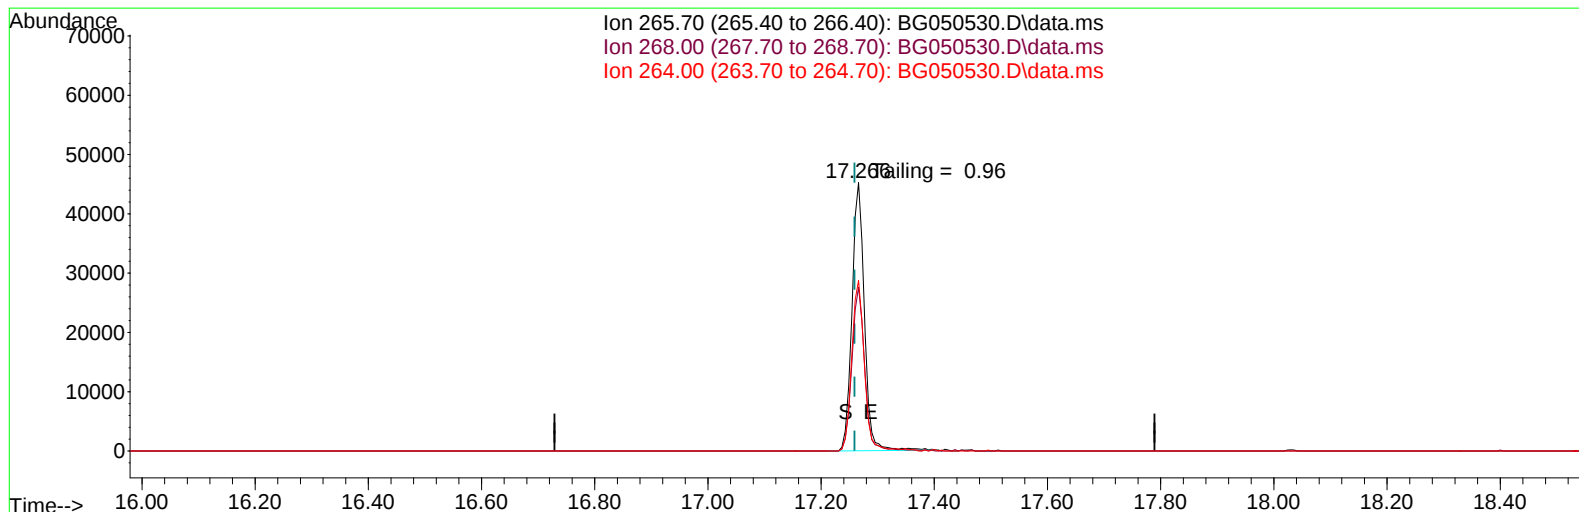

TIC: BG050530.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.007) 25289.66 ng




response 68451

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.08
264.00	61.30	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101121\
Data File : BG050530.D
Acq On : 11 Oct 2021 8:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 11 11:11:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

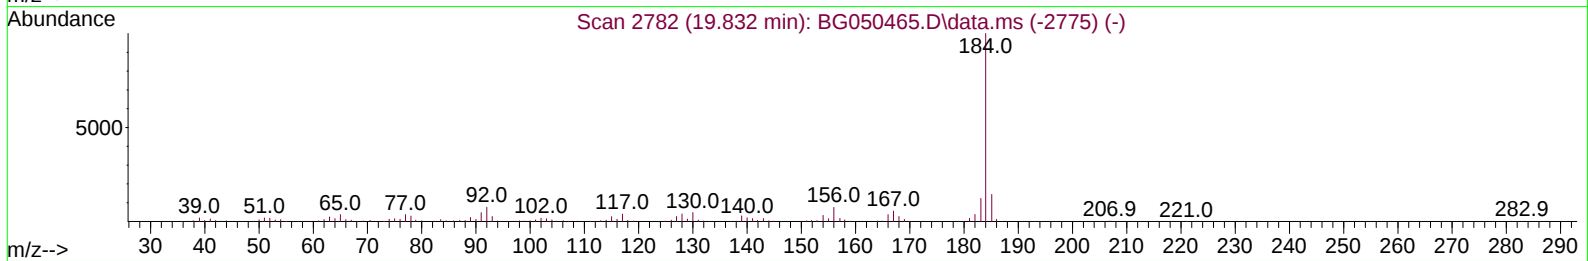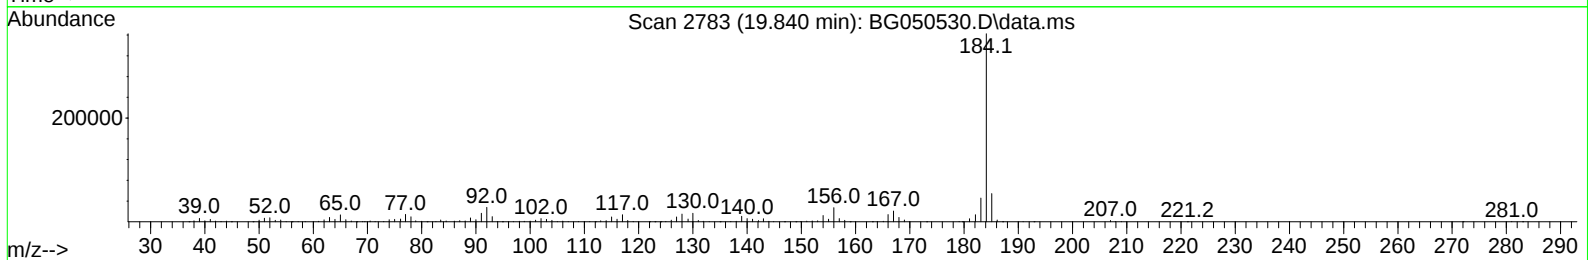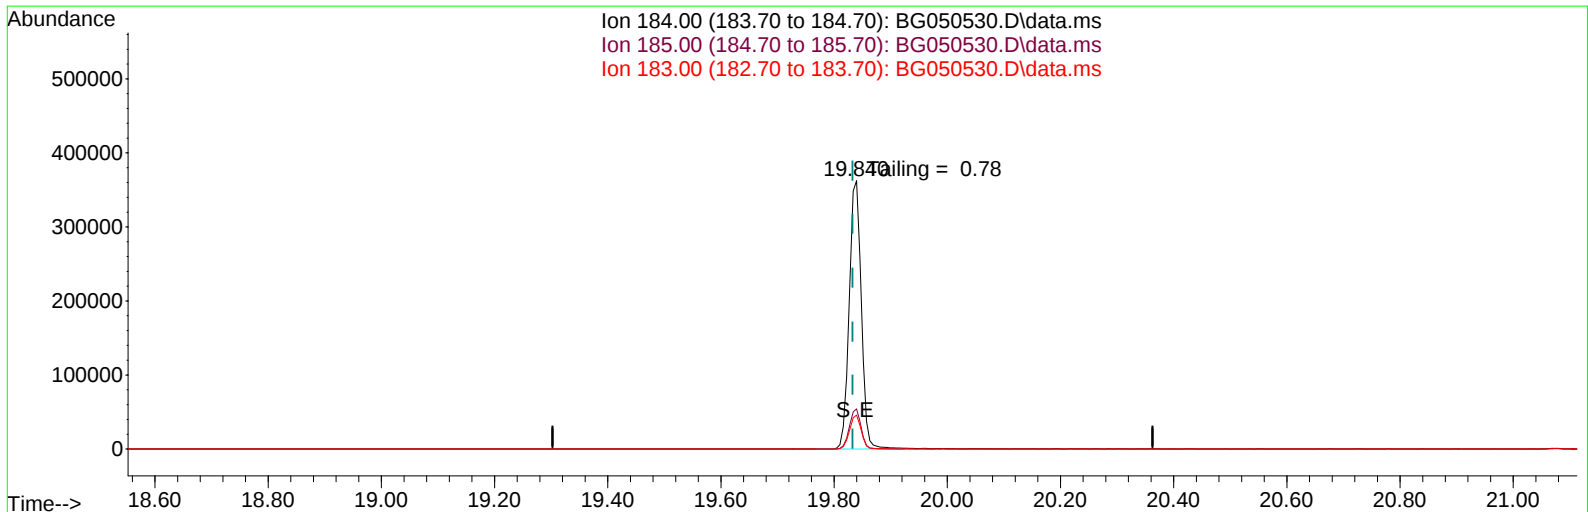

TIC: BG050530.D\data.ms

(77) Benzidine

19.840min (+ 0.007) 280898.07 ng

response 537150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.99
183.00	11.70	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2021	BNA_G	BG050530.D
Compound Name	Response	Retention Time
DDT	230958	21.07
DDD	8152	20.62
DDE	0	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8152	239110	3.41