
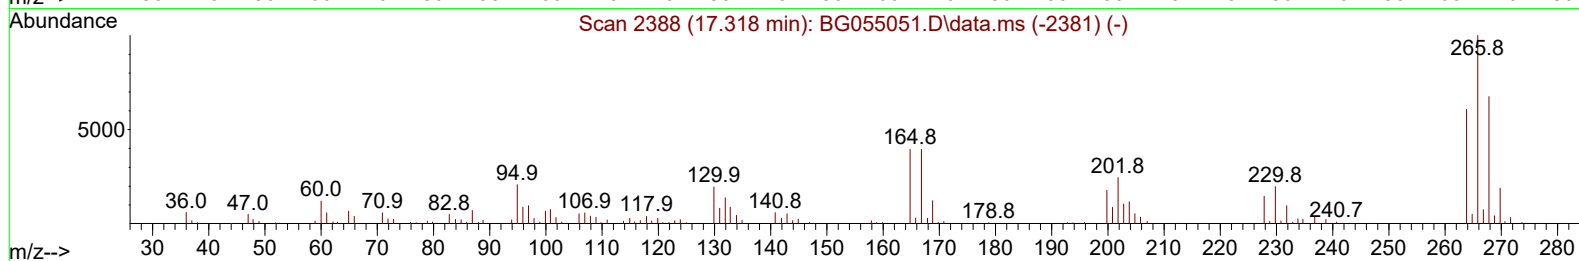
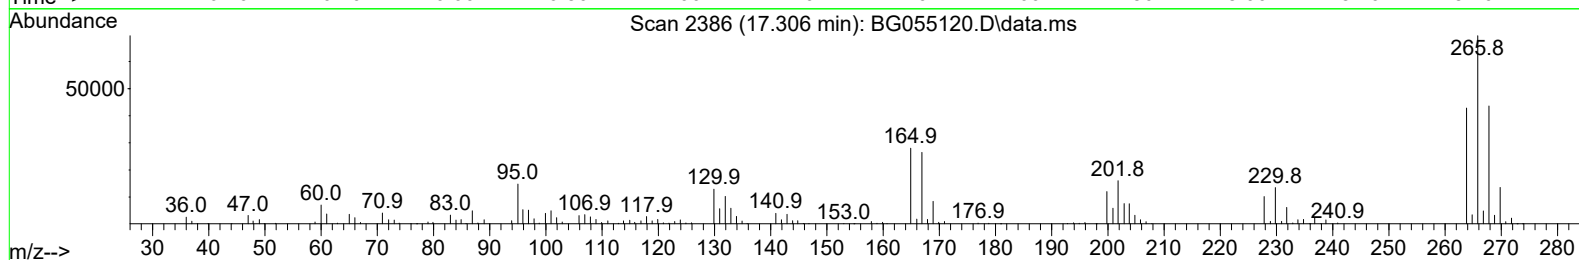


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101122\  
Data File : BG055120.D  
Acq On    : 11 Oct 2022    9:26  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Oct 12 08:05:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

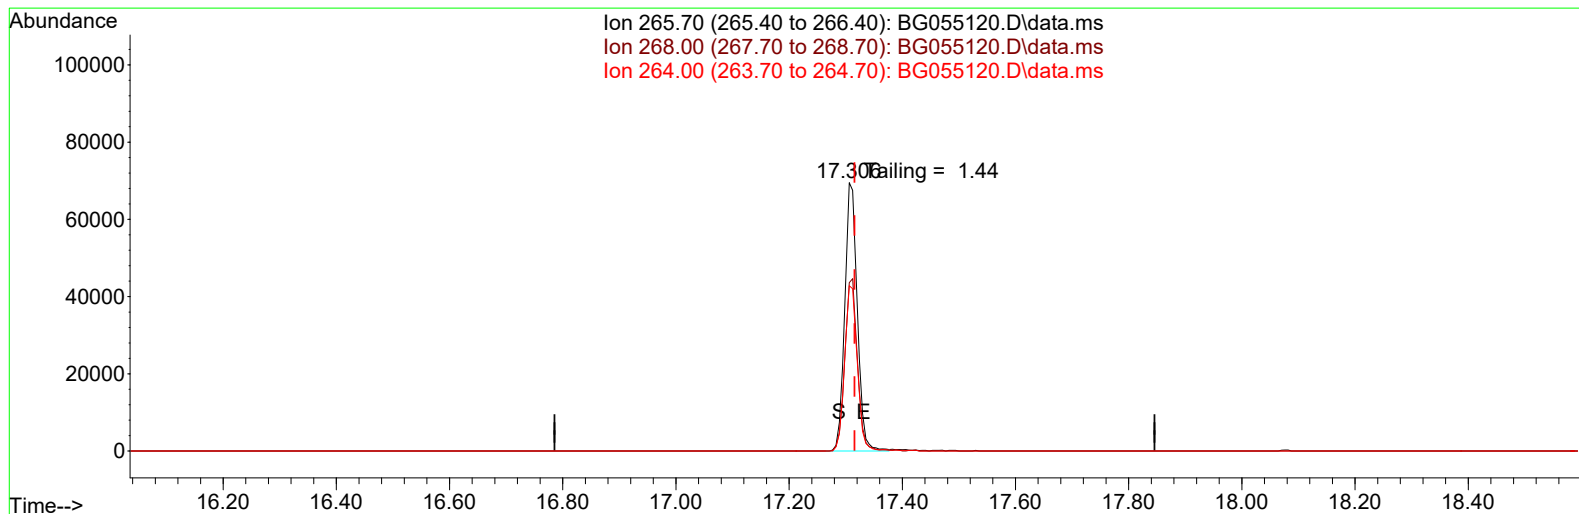

TIC: BG055120.D\data.ms

(70) Pentachlorophenol (C)




17.306min (-0.009) 33486.43 ng

response **107380**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.70
264.00	60.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101122\
Data File : BG055120.D
Acq On : 11 Oct 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:05:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

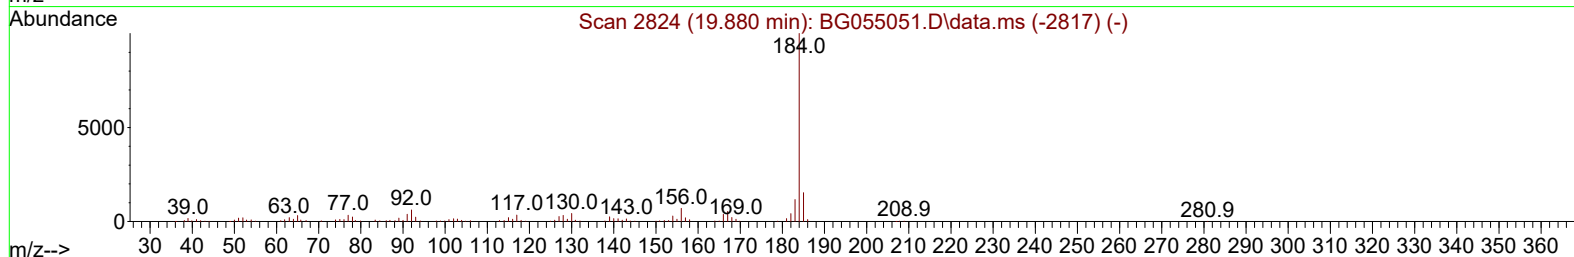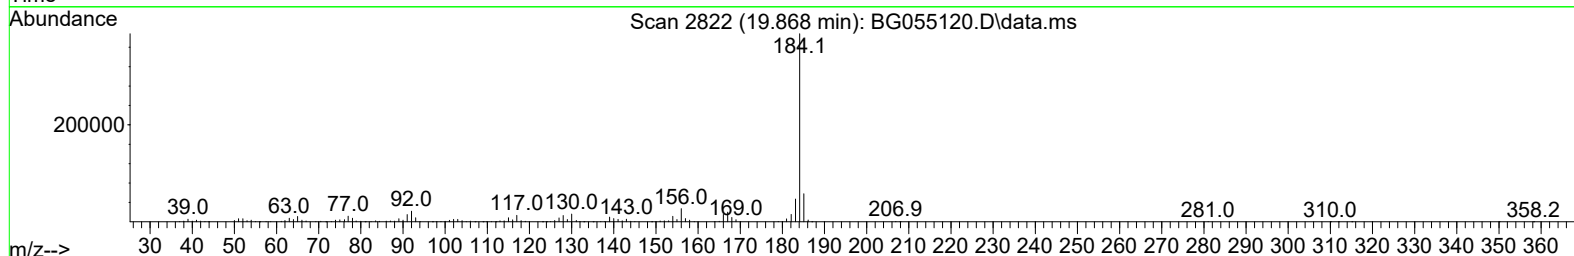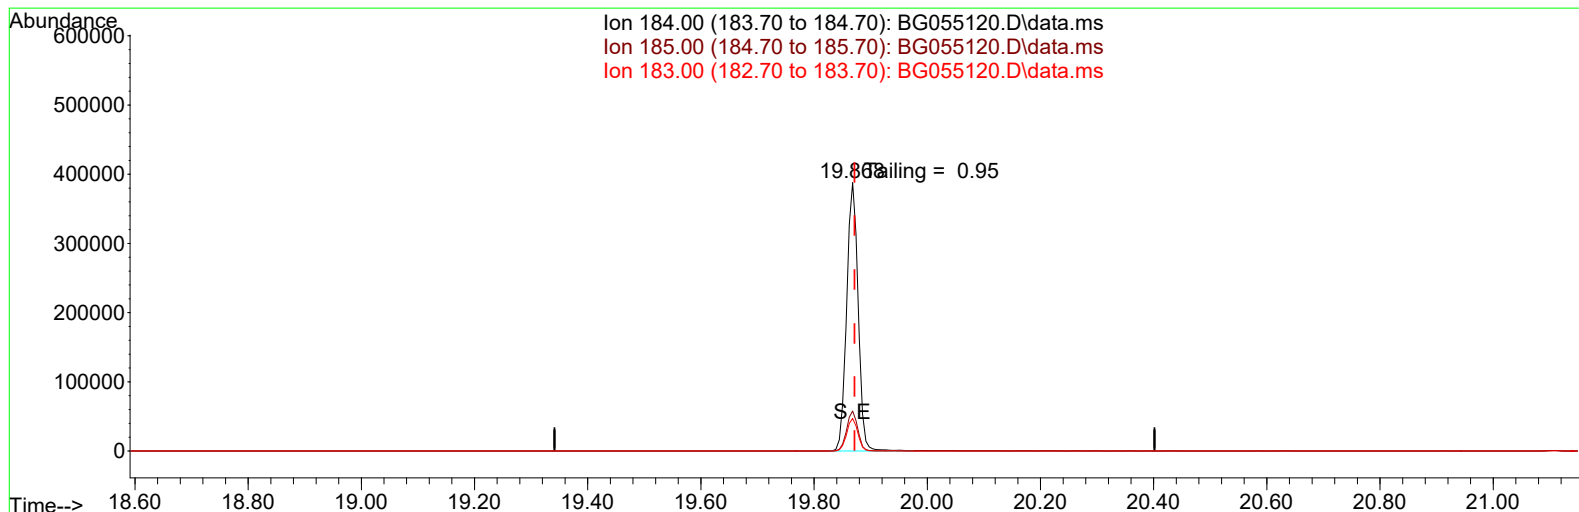

TIC: BG055120.D\data.ms

(77) Benzidine**19.868min (-0.003) 517538.13 ng****response 543857**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.91
183.00	11.70	12.13
0.00	0.00	0.00