
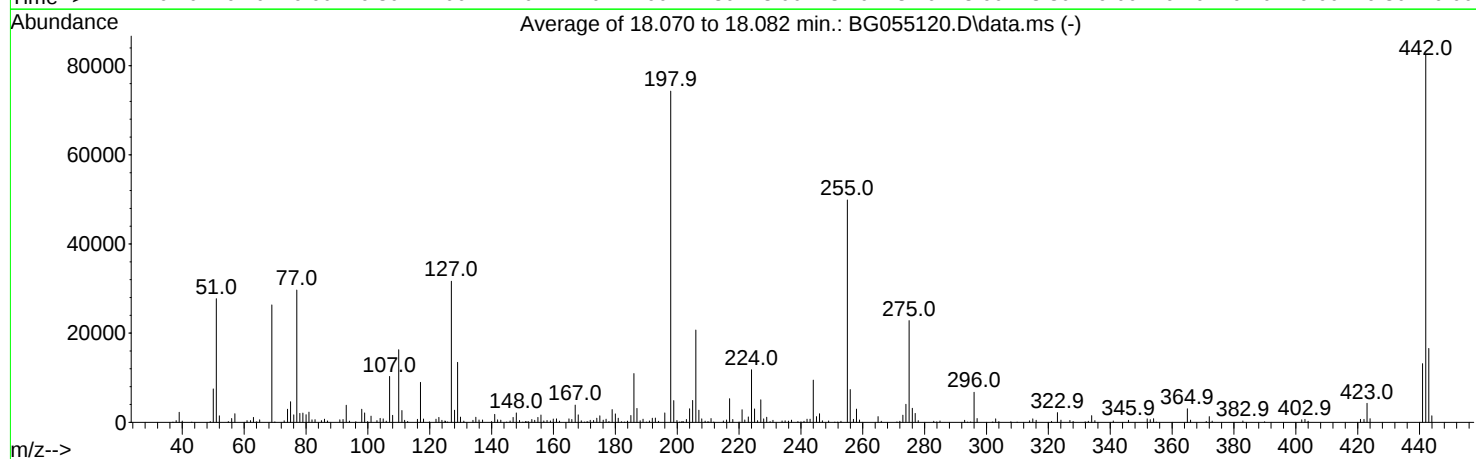


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101122\
 Data File : BG055120.D
 Acq On : 11 Oct 2022 9:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 08 03:04:59 2022

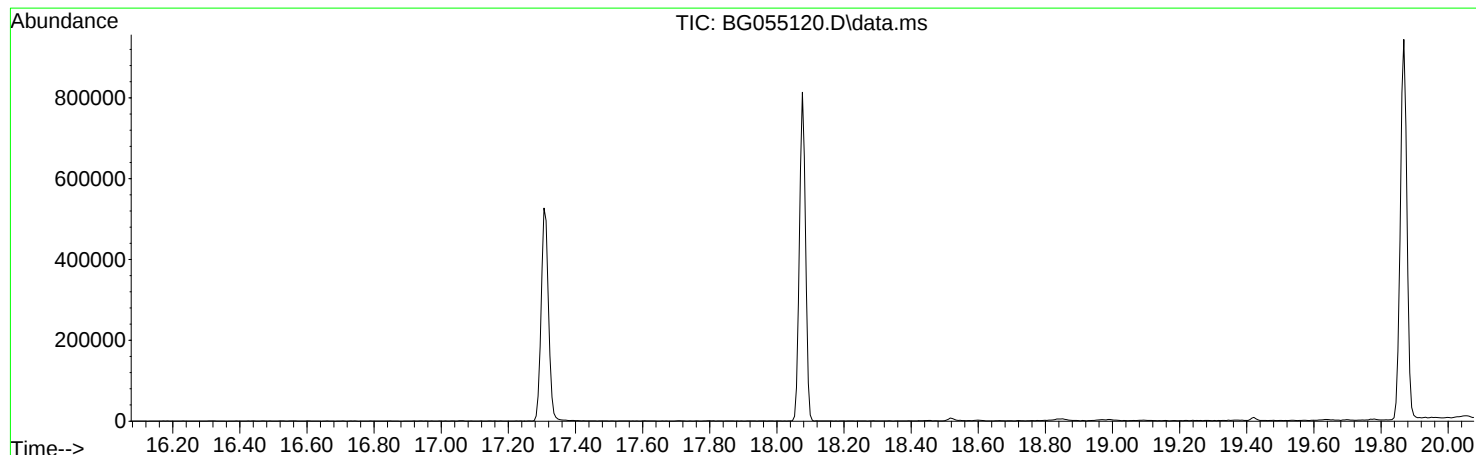




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	27755	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.5	26349	PASS
70	69	0.00	2	0.4	106	PASS
127	198	10	80	42.6	31645	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74288	PASS
199	198	5	9	6.6	4879	PASS
275	198	10	60	30.7	22821	PASS
365	198	1	100	4.1	3020	PASS
441	198	0.01	100	17.7	13166	PASS
442	442	50	100	100.0	82539	PASS
443	442	15	24	20.1	16579	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101122\
Data File : BG055120.D
Acq On : 11 Oct 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 12 08:05:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

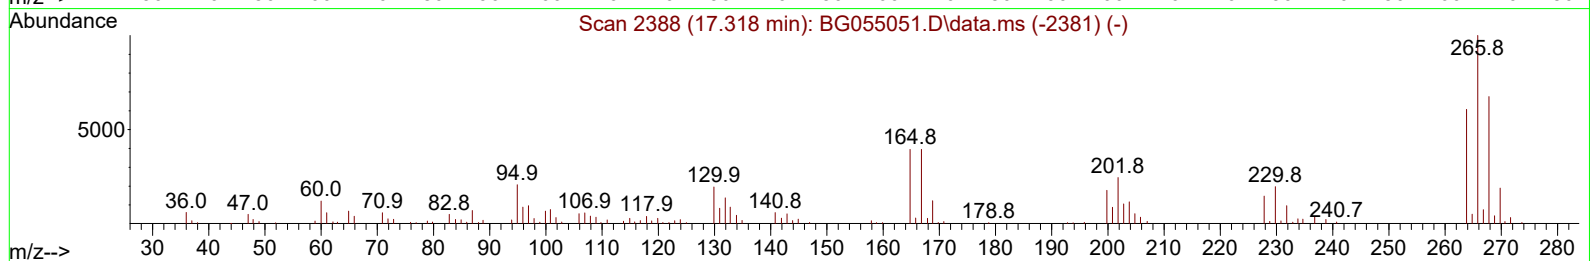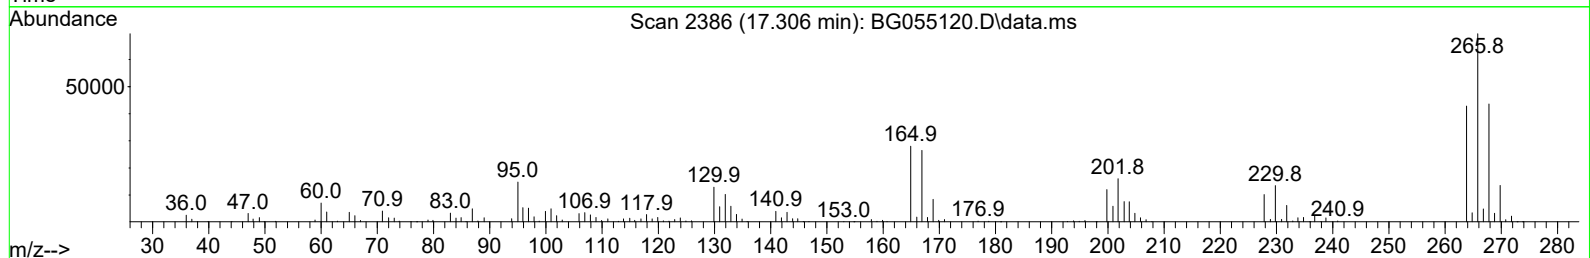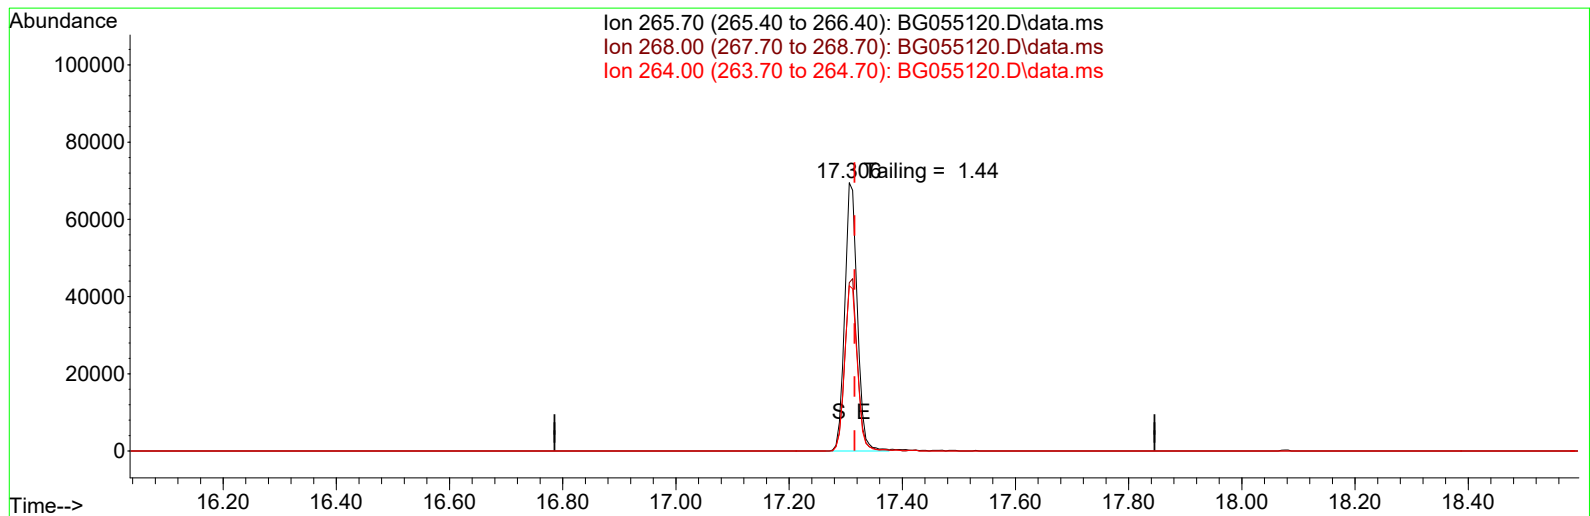

TIC: BG055120.D\data.ms

(70) Pentachlorophenol (C)

17.306min (-0.009) 33486.43 ng




response 107380

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	62.70
264.00	60.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101122\
Data File : BG055120.D
Acq On : 11 Oct 2022 9:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 12 08:05:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

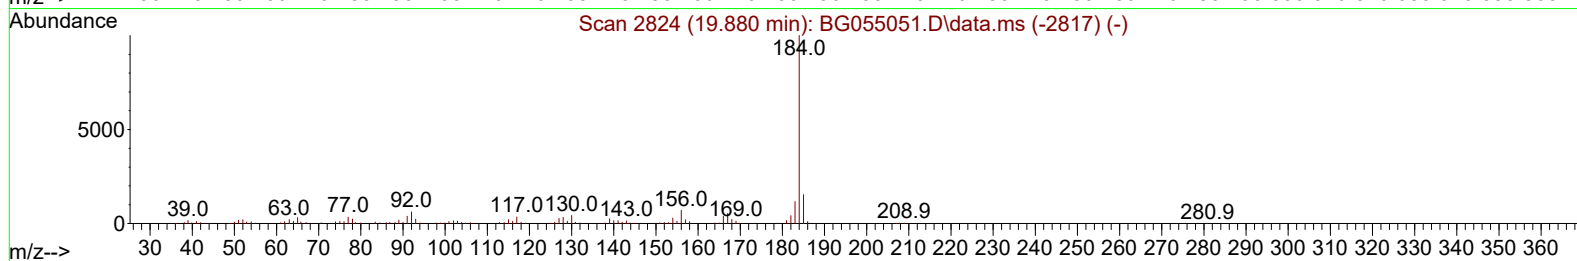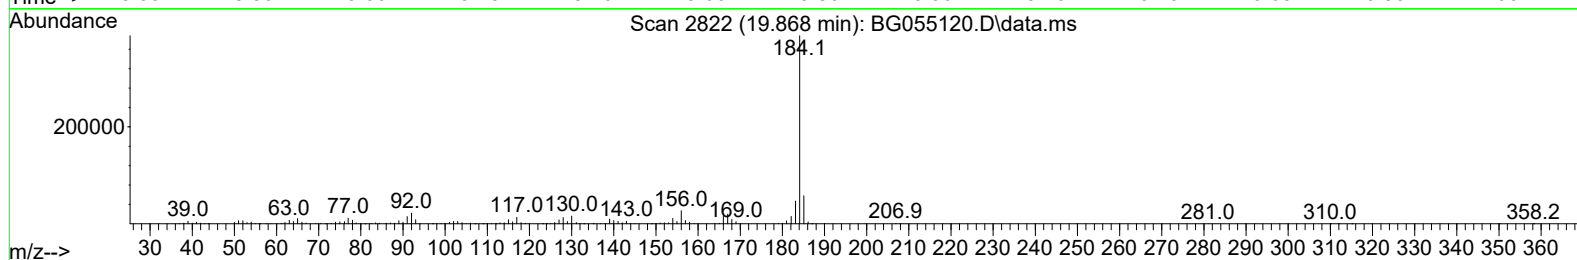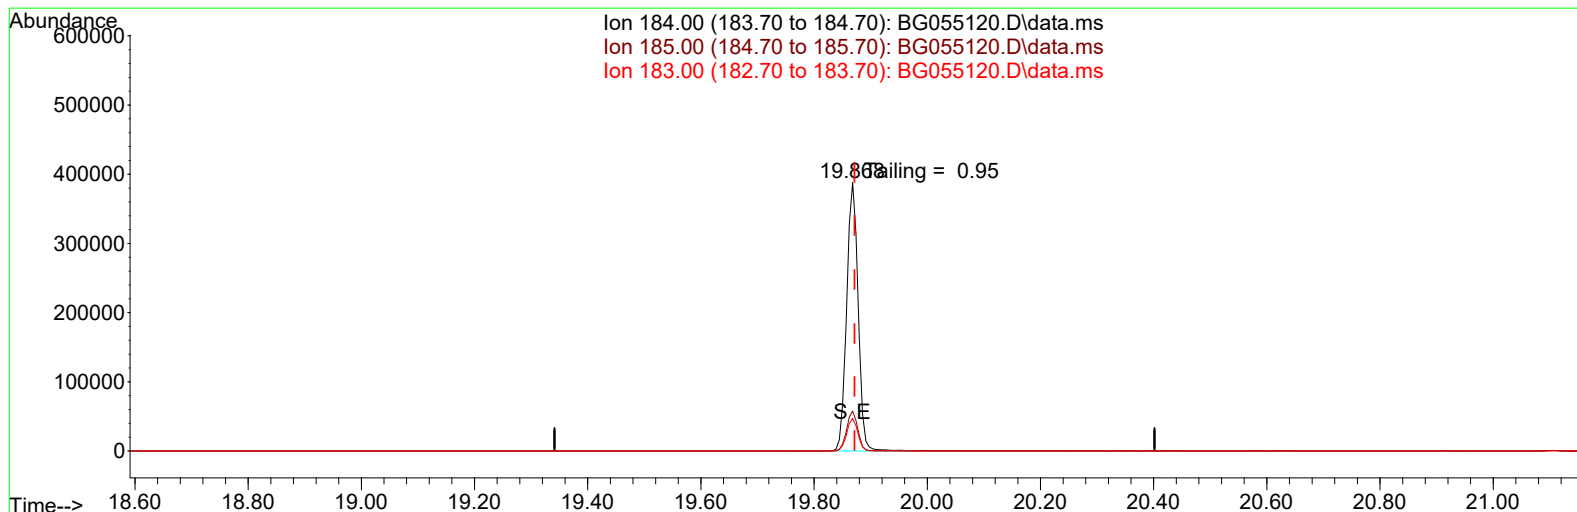

TIC: BG055120.D\data.ms

(77) Benzidine

19.868min (-0.003) 517538.13 ng

response 543857

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.91
183.00	11.70	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2022	BNA_G	<u>BG055120.D</u>
Compound Name	Response	Retention Time
DDT	248516	21.108
DDD	8135	20.649
DDE	85	20.15
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8220	256736	3.20

Instrument :
BNA_G
ClientSampleId :
DFTPP