
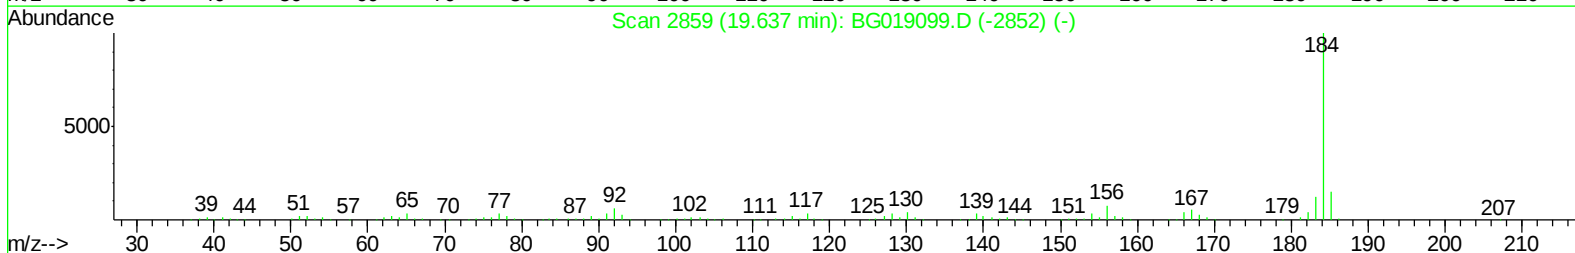
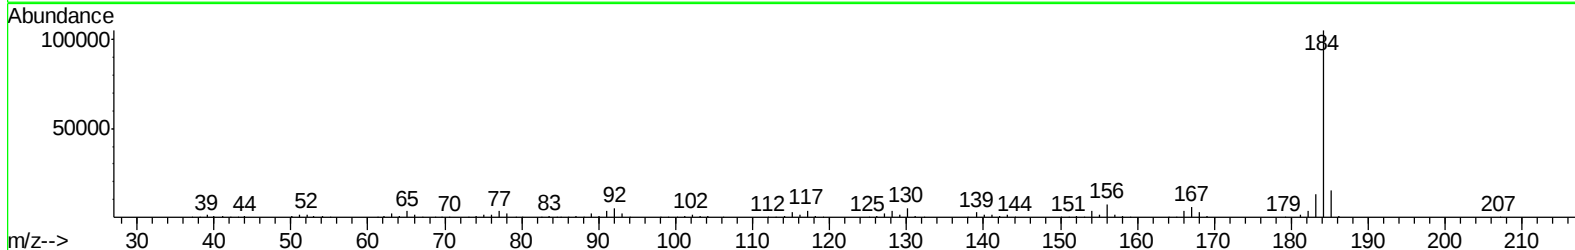


Data Path : Z:\HPCHEM1\BNA G\Data\BG101215\
Data File : BG019148.D
Acq On : 12 Oct 2015 4:52
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:54:56 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 07:23:23 2015
Response via : Initial Calibration

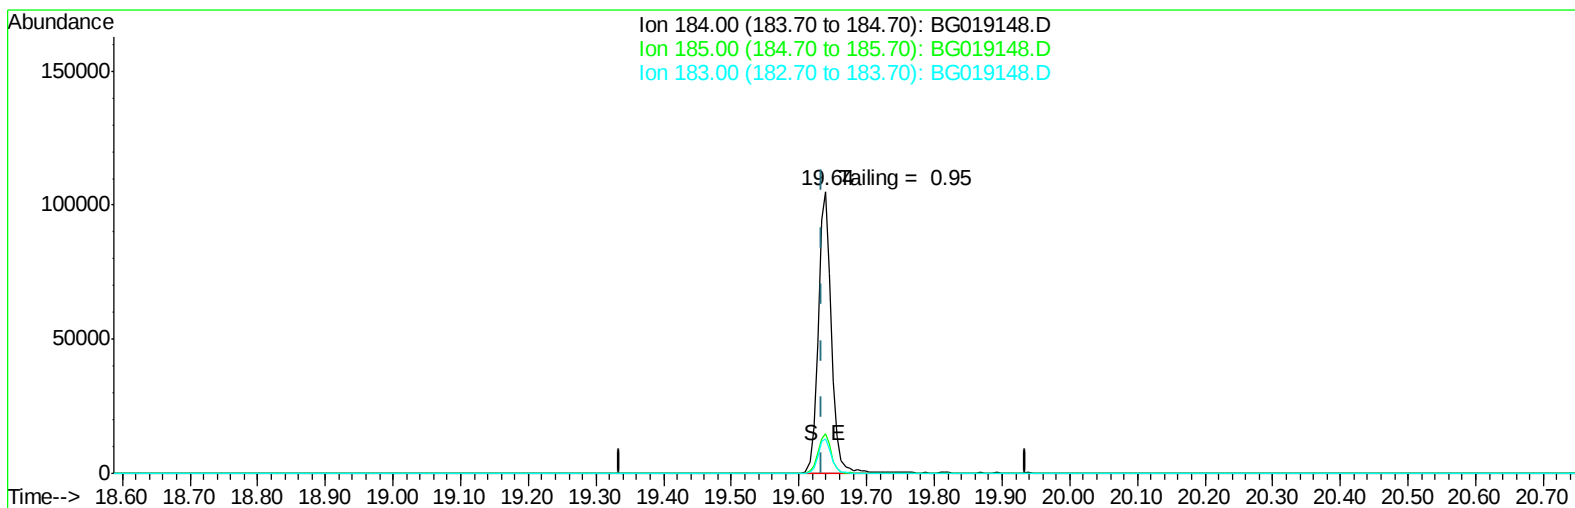

TIC: BG019148.D

(76) Benzidine




19.639min (+0.004) 0.00ng

response 144580

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	14.20
183.00	12.60	12.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG101215\
Data File : BG019148.D
Acq On : 12 Oct 2015 4:52
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 07:54:56 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 07:23:23 2015
Response via : Initial Calibration

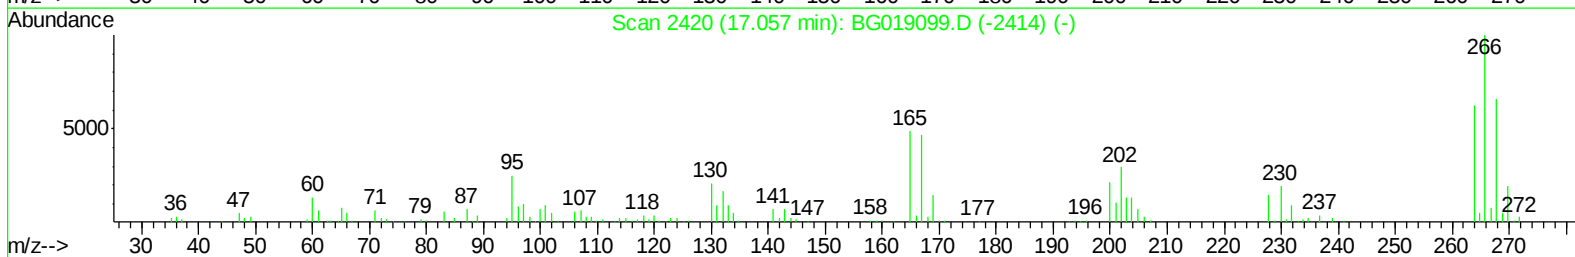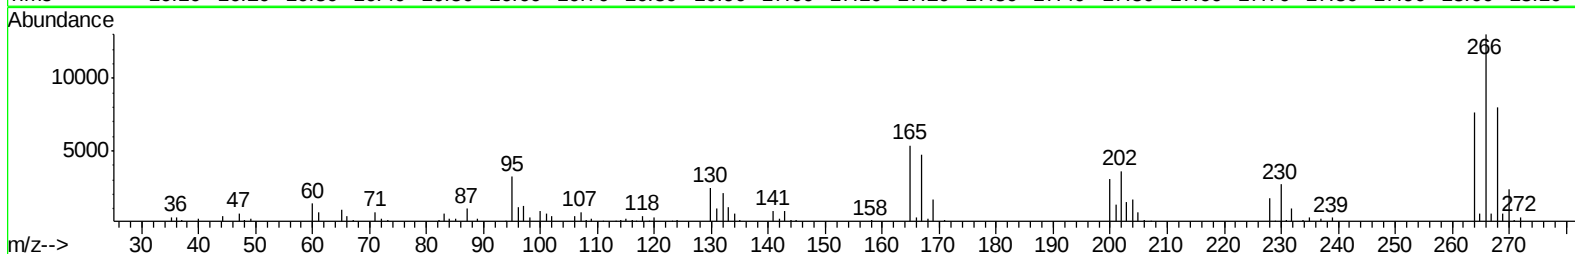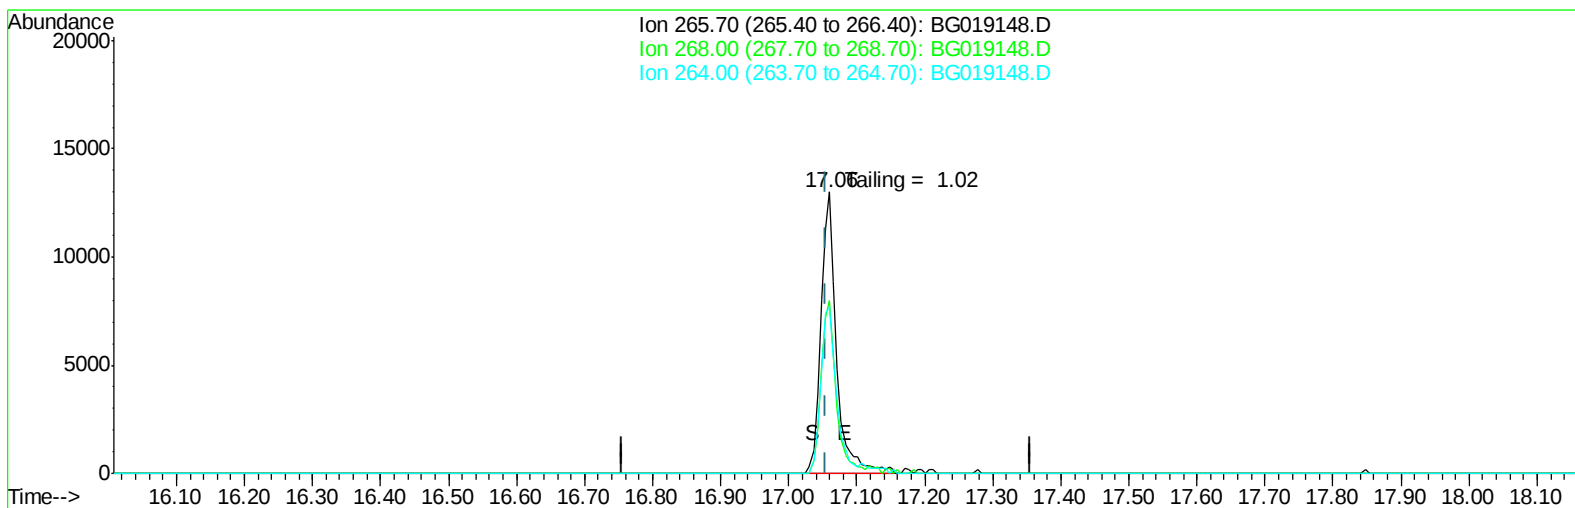

TIC: BG019148.D

(69) Pentachlorophenol (C)

17.060min (+0.004) 0.00ng

response 21105

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	61.43
264.00	62.60	58.91
0.00	0.00	0.00