


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101215\
 Data File : BG019148.D
 Acq On : 12 Oct 2015 4:52
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 10 07:04:31 2015

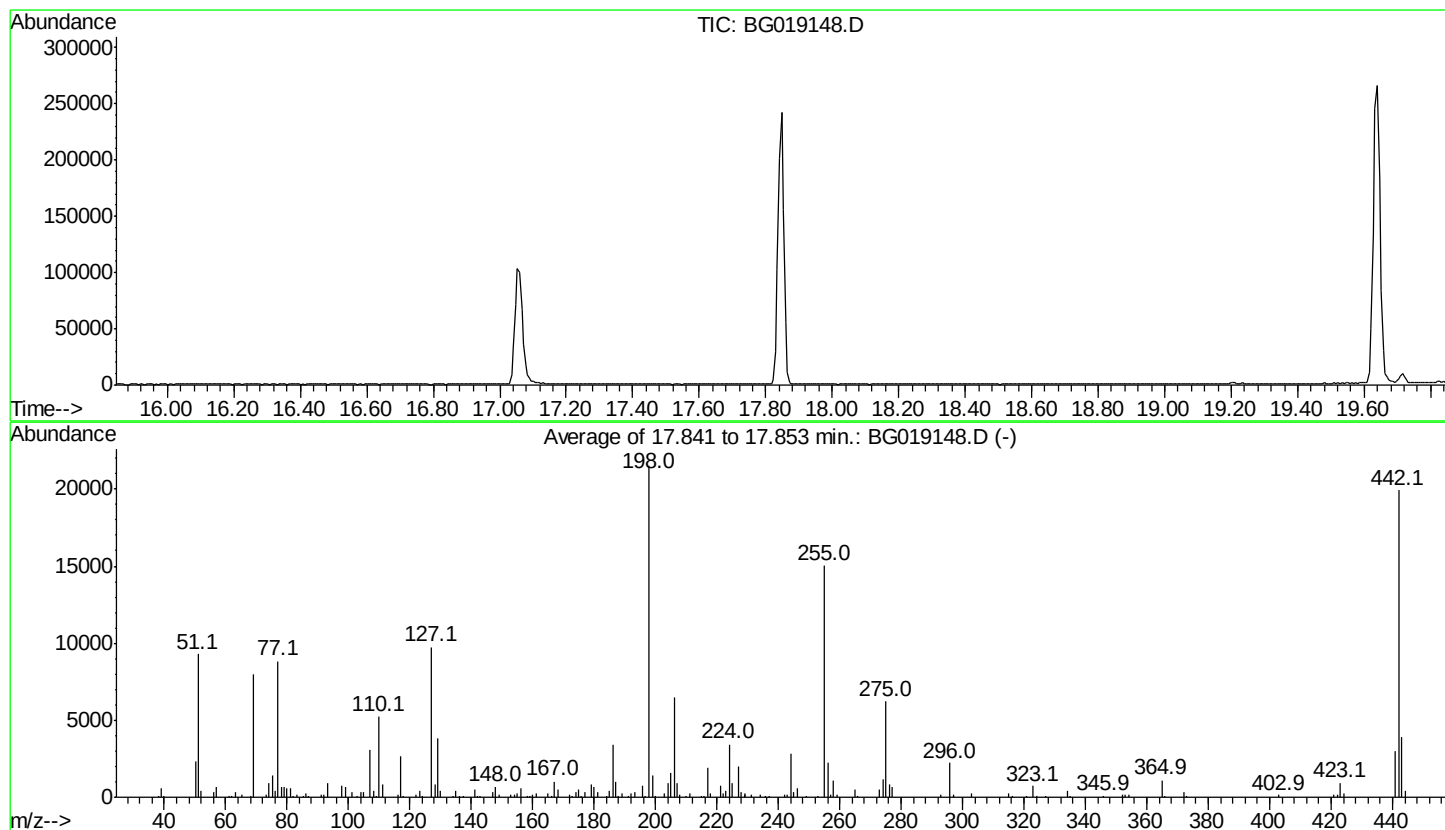

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	9302	PASS
68	69	0.00	2	0.9	74	PASS
69	198	0.00	100	37.2	8004	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	9754	PASS
197	198	0.00	2	0.5	105	PASS
198	198	100	100	100.0	21528	PASS
199	198	5	9	6.7	1435	PASS
275	198	10	60	28.9	6221	PASS
365	198	1	100	5.1	1092	PASS
441	442	0.01	24	15.0	2982	PASS
442	198	50	100	92.6	19933	PASS
443	442	15	24	19.5	3889	PASS