

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101216\
 Data File : BG024309.D
 Acq On : 12 Oct 2016 20:07
 Operator : UM/SJ
 Sample : H5145-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDN95

Quant Time: Oct 13 01:34:24 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 01:34:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	139387	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	627908	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	528514	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1110090	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1243271	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1268616	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	8773	2.99	ng/uL	0.00
5) Phenol-d5	7.41	99	214873	16.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	155777	17.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	161279	18.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	159163	15.14	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	82884	18.60	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	101075	20.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	191543	17.64	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	248548	21.79	ng/ul	0.00
43) Dimethylphthalate-d6	14.29	166	714718	19.37	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	837143	19.80	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	108788	16.63	ng/ul	0.00
57) Fluorene-d10	15.89	176	694644	19.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	110040	16.49	ng/ul	0.00
70) Anthracene-d10	17.74	188	1035371	20.65	ng/ul	0.00
76) Pyrene-d10	20.01	212	1199875	20.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.14	264	1214073	21.27	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.34	163	346094	9.56	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101216\
Data File : BG024309.D
Acq On : 12 Oct 2016 20:07
Operator : UM/SJ
Sample : H5145-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDN95

Quant Time: Oct 13 01:34:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 01:34:23 2016
Response via : Initial Calibration

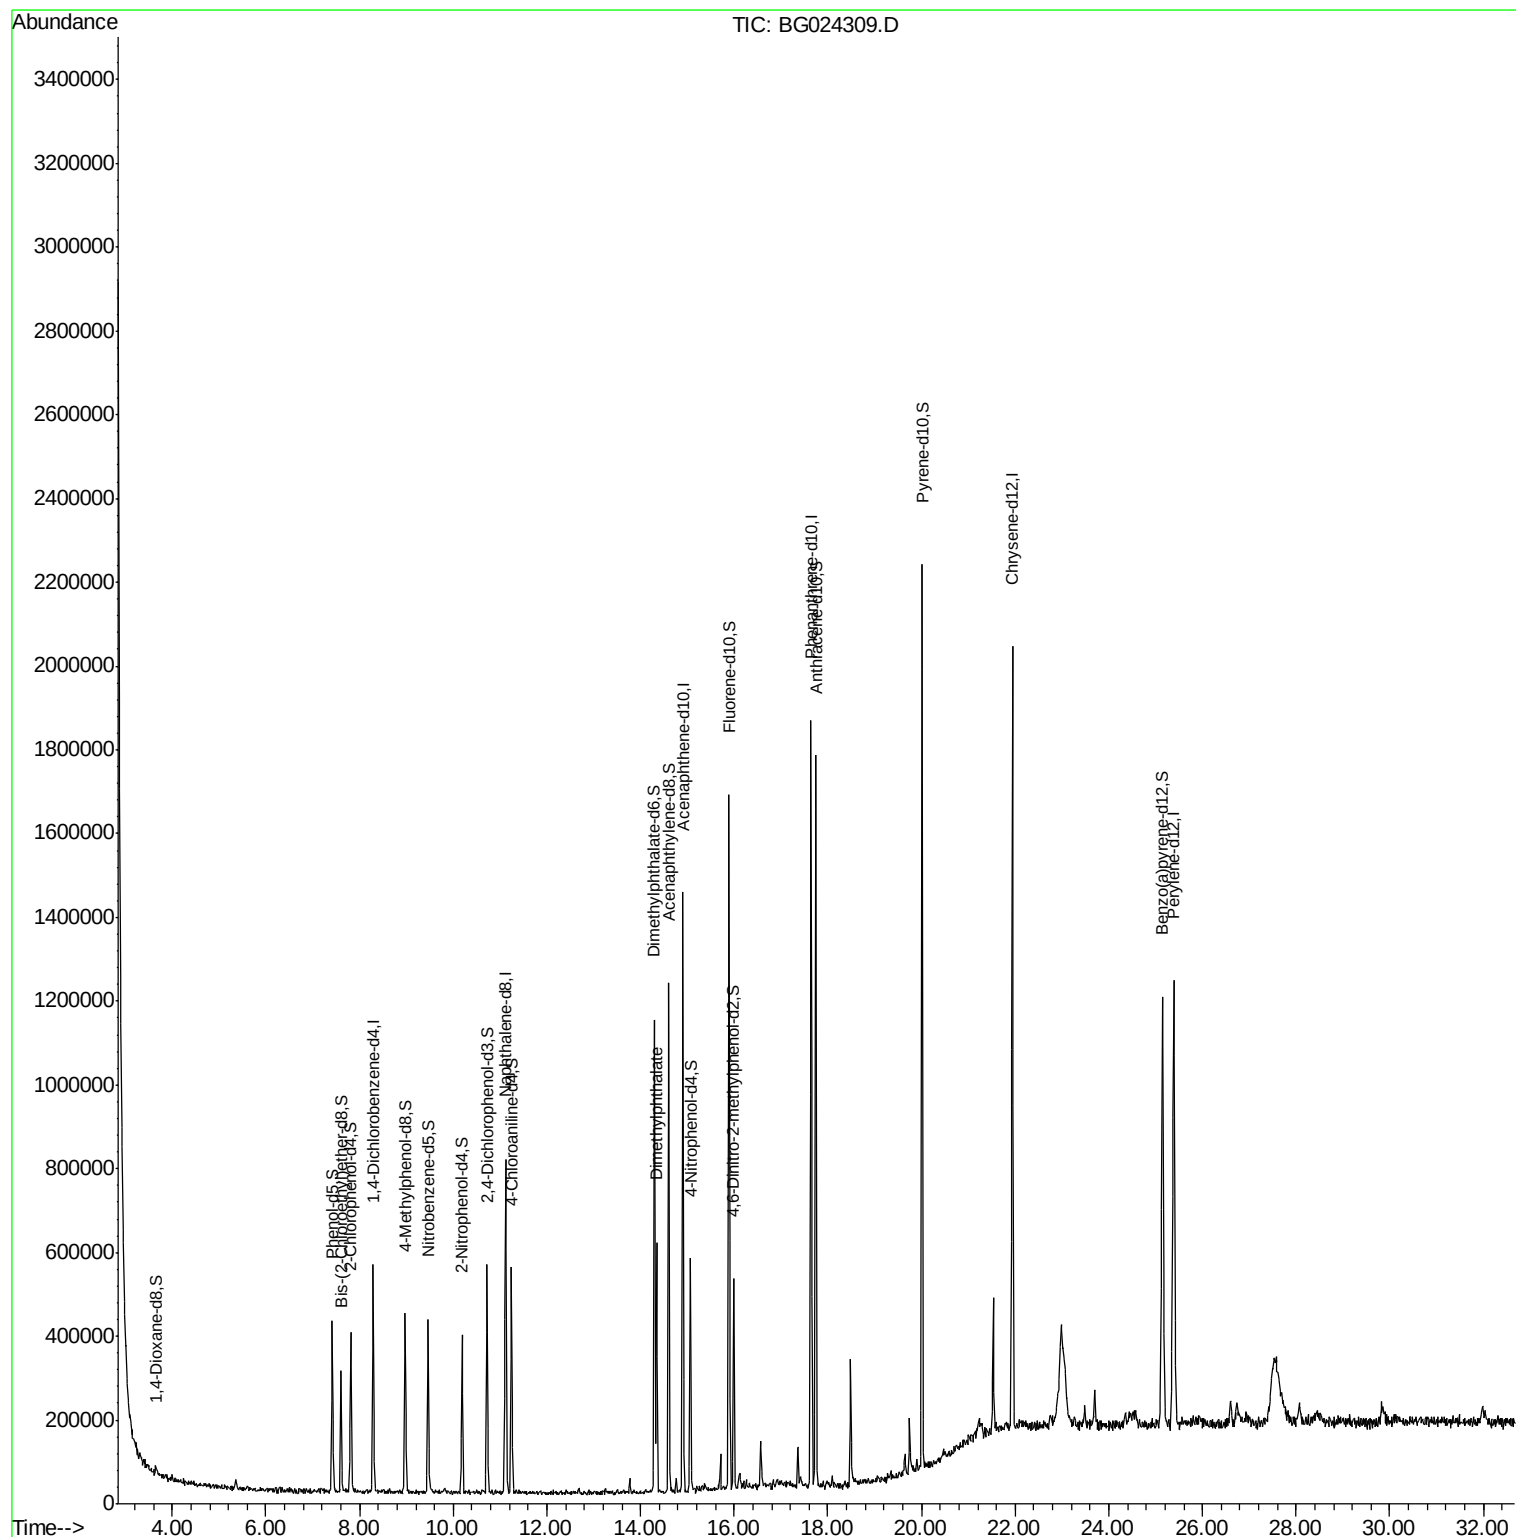

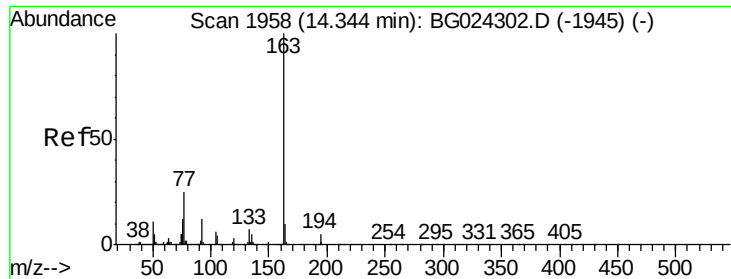

#44

Dimethylphthalate

Concen: 9.56 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. -0.00 min

Lab File: BG024309.D

Acq: 12 Oct 2016 20:07

Instrument :

BNA_G

ClientSampleId :

BDN95

Tgt Ion:163 Resp: 346094

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.0

164 12.2 9.0 13.4

