


Data Path : Z:\HPCHEM1\BNA_G\Data\BG101217\
 Data File : BG029165.D
 Acq On : 11 Oct 2017 14:40
 Operator : SJ/JU
 Sample : DFTPP55
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP55

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG100717MA.M
 Title : SVOA CALIBRATION
 Last Update : Wed Oct 11 04:15:46 2017

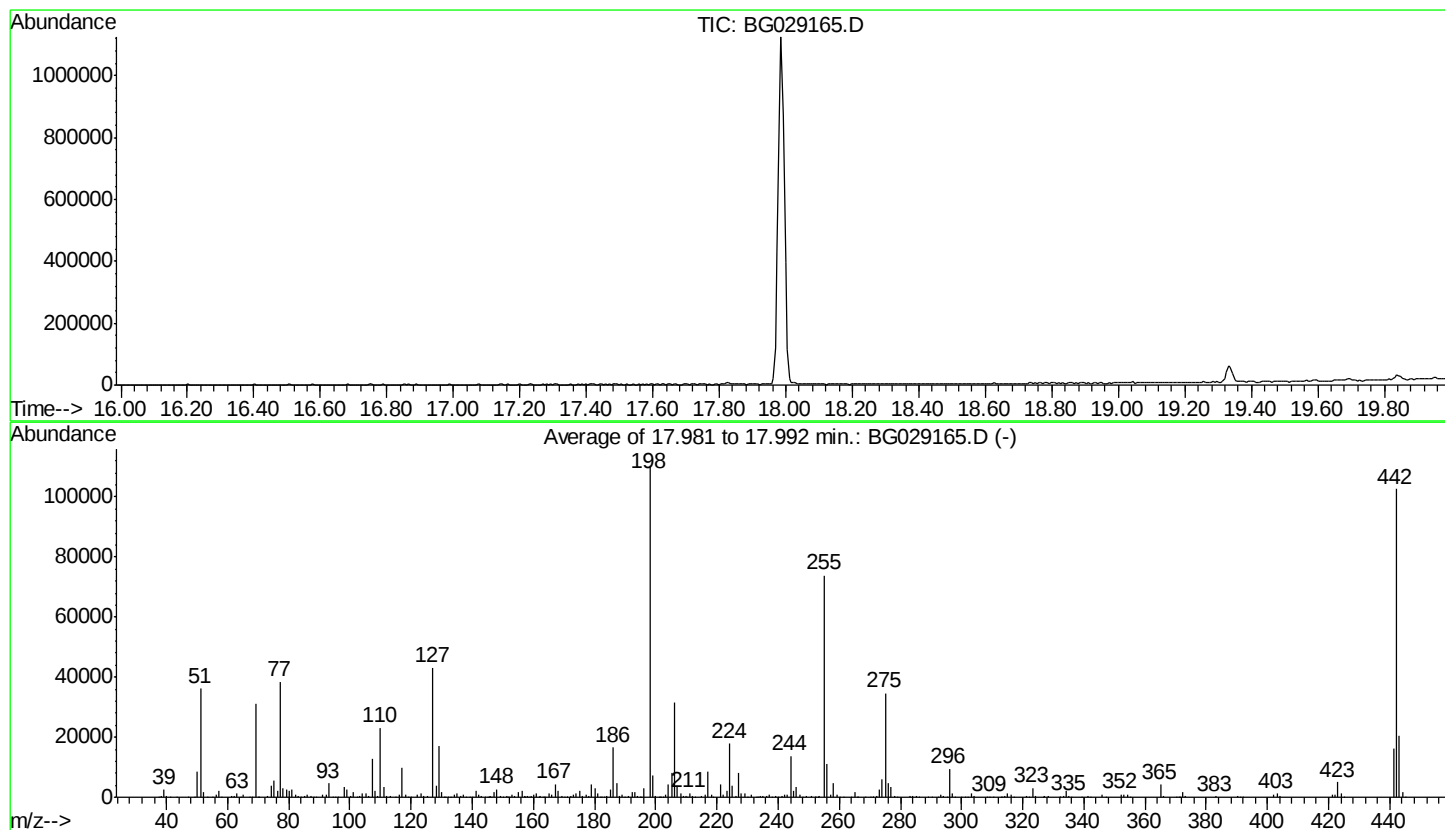

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	36197	PASS
68	69	0.00	2	0.7	209	PASS
69	198	0.00	100	28.1	31078	PASS
70	69	0.00	2	0.3	92	PASS
127	198	10	80	39.2	43272	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110456	PASS
199	198	5	9	6.7	7393	PASS
275	198	10	60	31.3	34576	PASS
365	198	1	100	3.8	4213	PASS
441	442	0.01	100	15.6	16045	PASS
442	198	50	100	93.0	102736	PASS
443	442	15	24	19.9	20495	PASS