
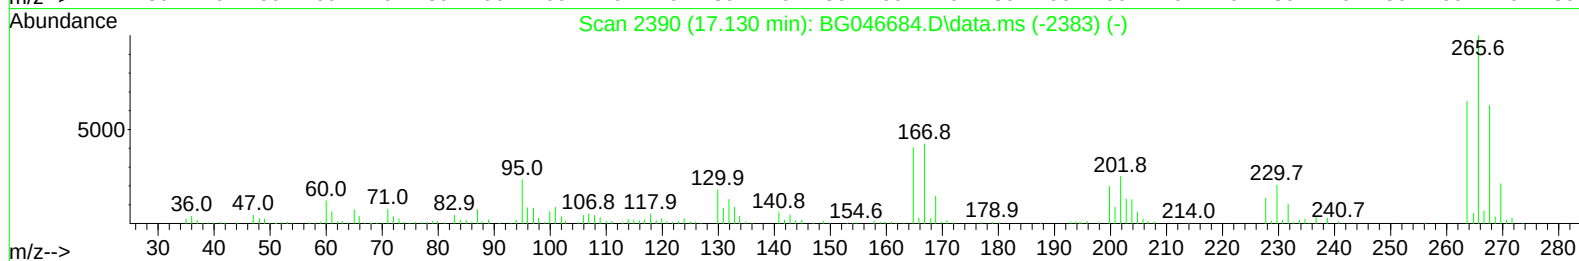
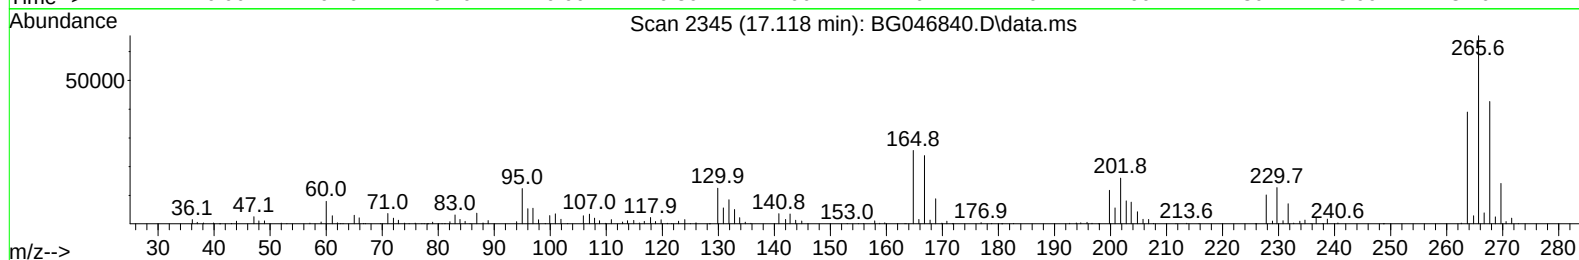


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
Data File : BG046840.D
Acq On : 12 Oct 2020 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 03:33:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

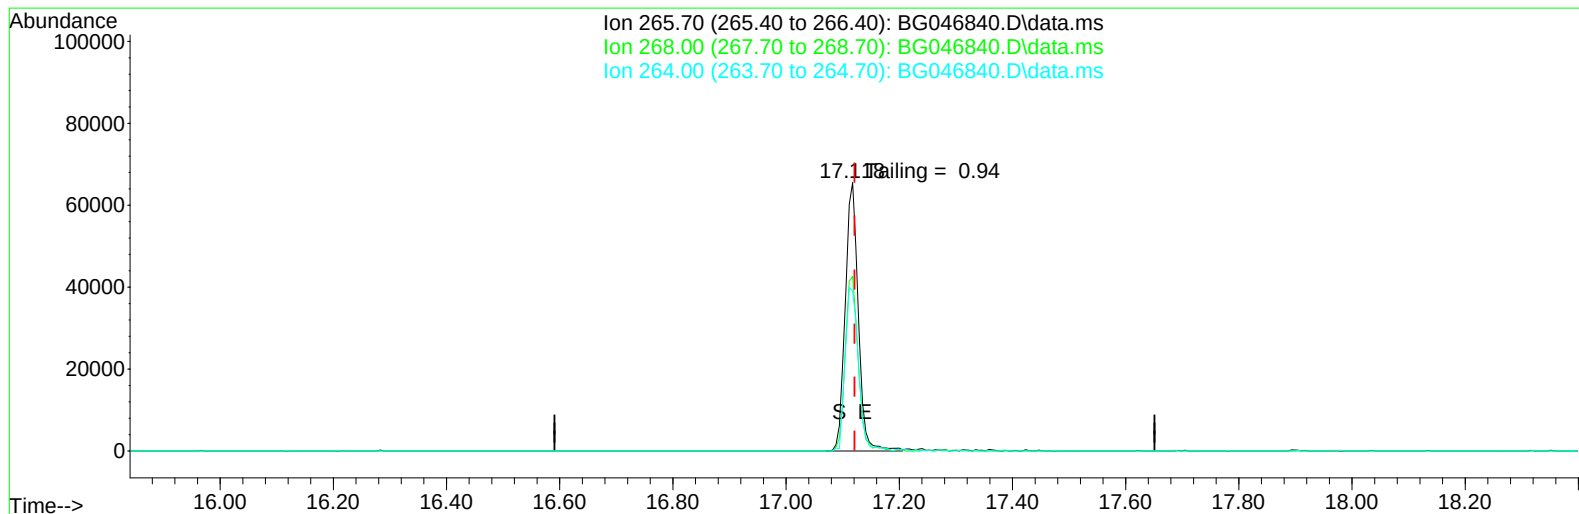

TIC: BG046840.D\data.ms

(70) Pentachlorophenol (C)




17.118min (-0.003) 150945.75 ng

response 105428

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.94
264.00	61.60	59.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
Data File : BG046840.D
Acq On : 12 Oct 2020 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 03:33:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

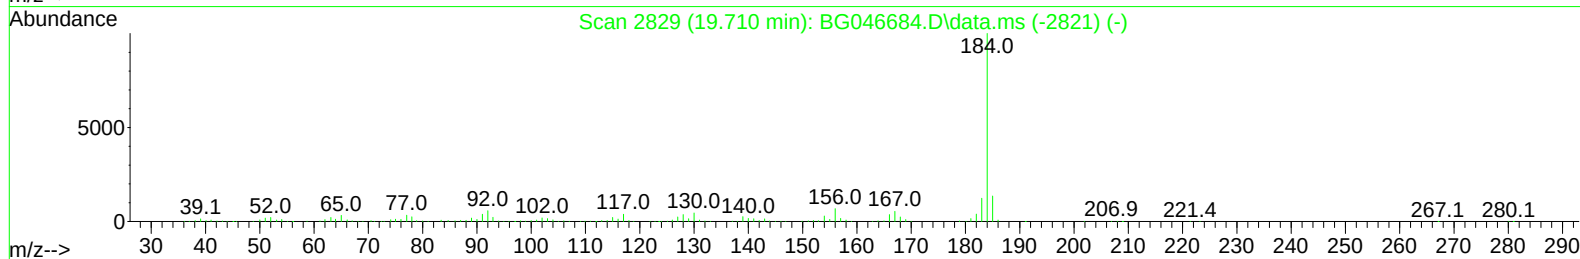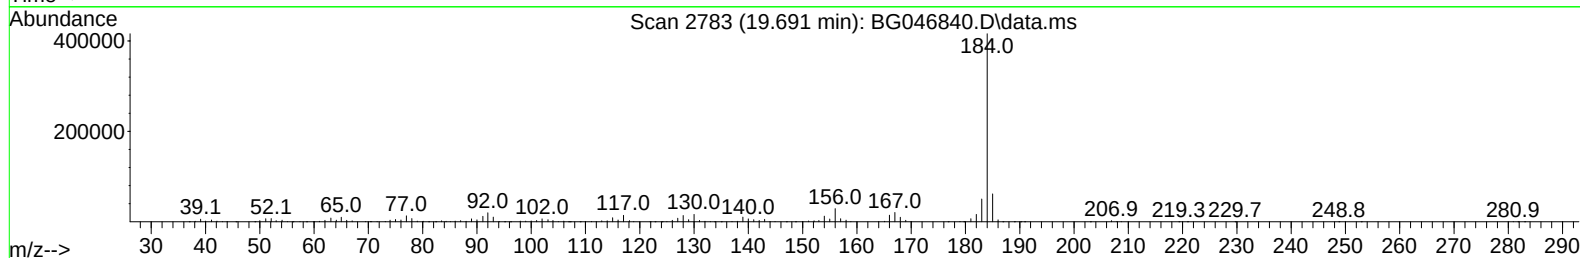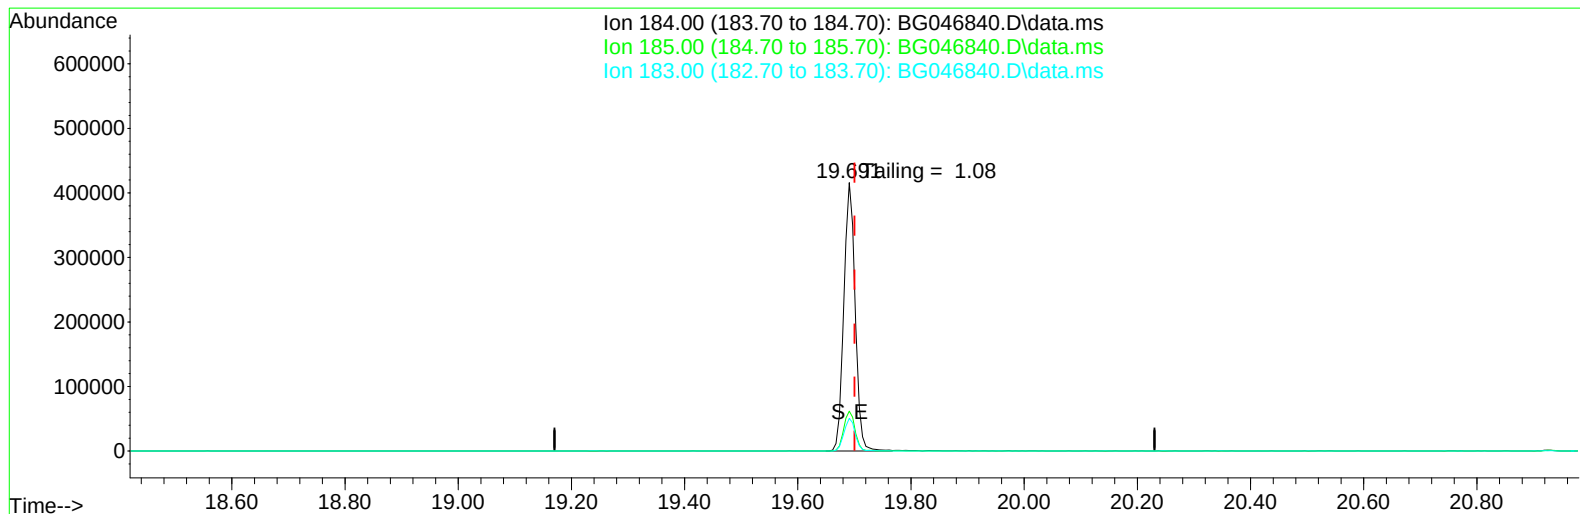

TIC: BG046840.D\data.ms

(77) Benzidine

19.691min (-0.009) 231737.12 ng

response 578614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.84
183.00	13.20	12.16
0.00	0.00	0.00