

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
 Data File : BG046861.D
 Acq On : 13 Oct 2020 3:48
 Operator : CG/JU
 Sample : PB132258TB
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB132258TB

Quant Time: Oct 13 04:39:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 07 11:38:17 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.106	152	55124	20.00	ng	# 0.00
21) Naphthalene-d8	10.915	136	206001	20.00	ng	# 0.00
39) Acenaphthene-d10	14.728	164	155429	20.00	ng	0.00
64) Phenanthrene-d10	17.466	188	456602	20.00	ng	#-0.01
76) Chrysene-d12	21.743	240	551070	20.00	ng	#-0.01
86) Perylene-d12	25.010	264	536257	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.668	112	524960	152.56	ng	0.00
7) Phenol-d6	7.254	99	680409	140.19	ng	0.00
23) Nitrobenzene-d5	9.264	82	477217	123.24	ng	0.00
42) 2,4,6-Tribromophenol	16.214	330	427779	208.73	ng	0.00
45) 2-Fluorobiphenyl	13.353	172	1121826	102.18	ng	0.00
79) Terphenyl-d14	20.074	244	2612189	95.00	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
Data File : BG046861.D
Acq On : 13 Oct 2020 3:48
Operator : CG/JU
Sample : PB132258TB
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB132258TB

Quant Time: Oct 13 04:39:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration




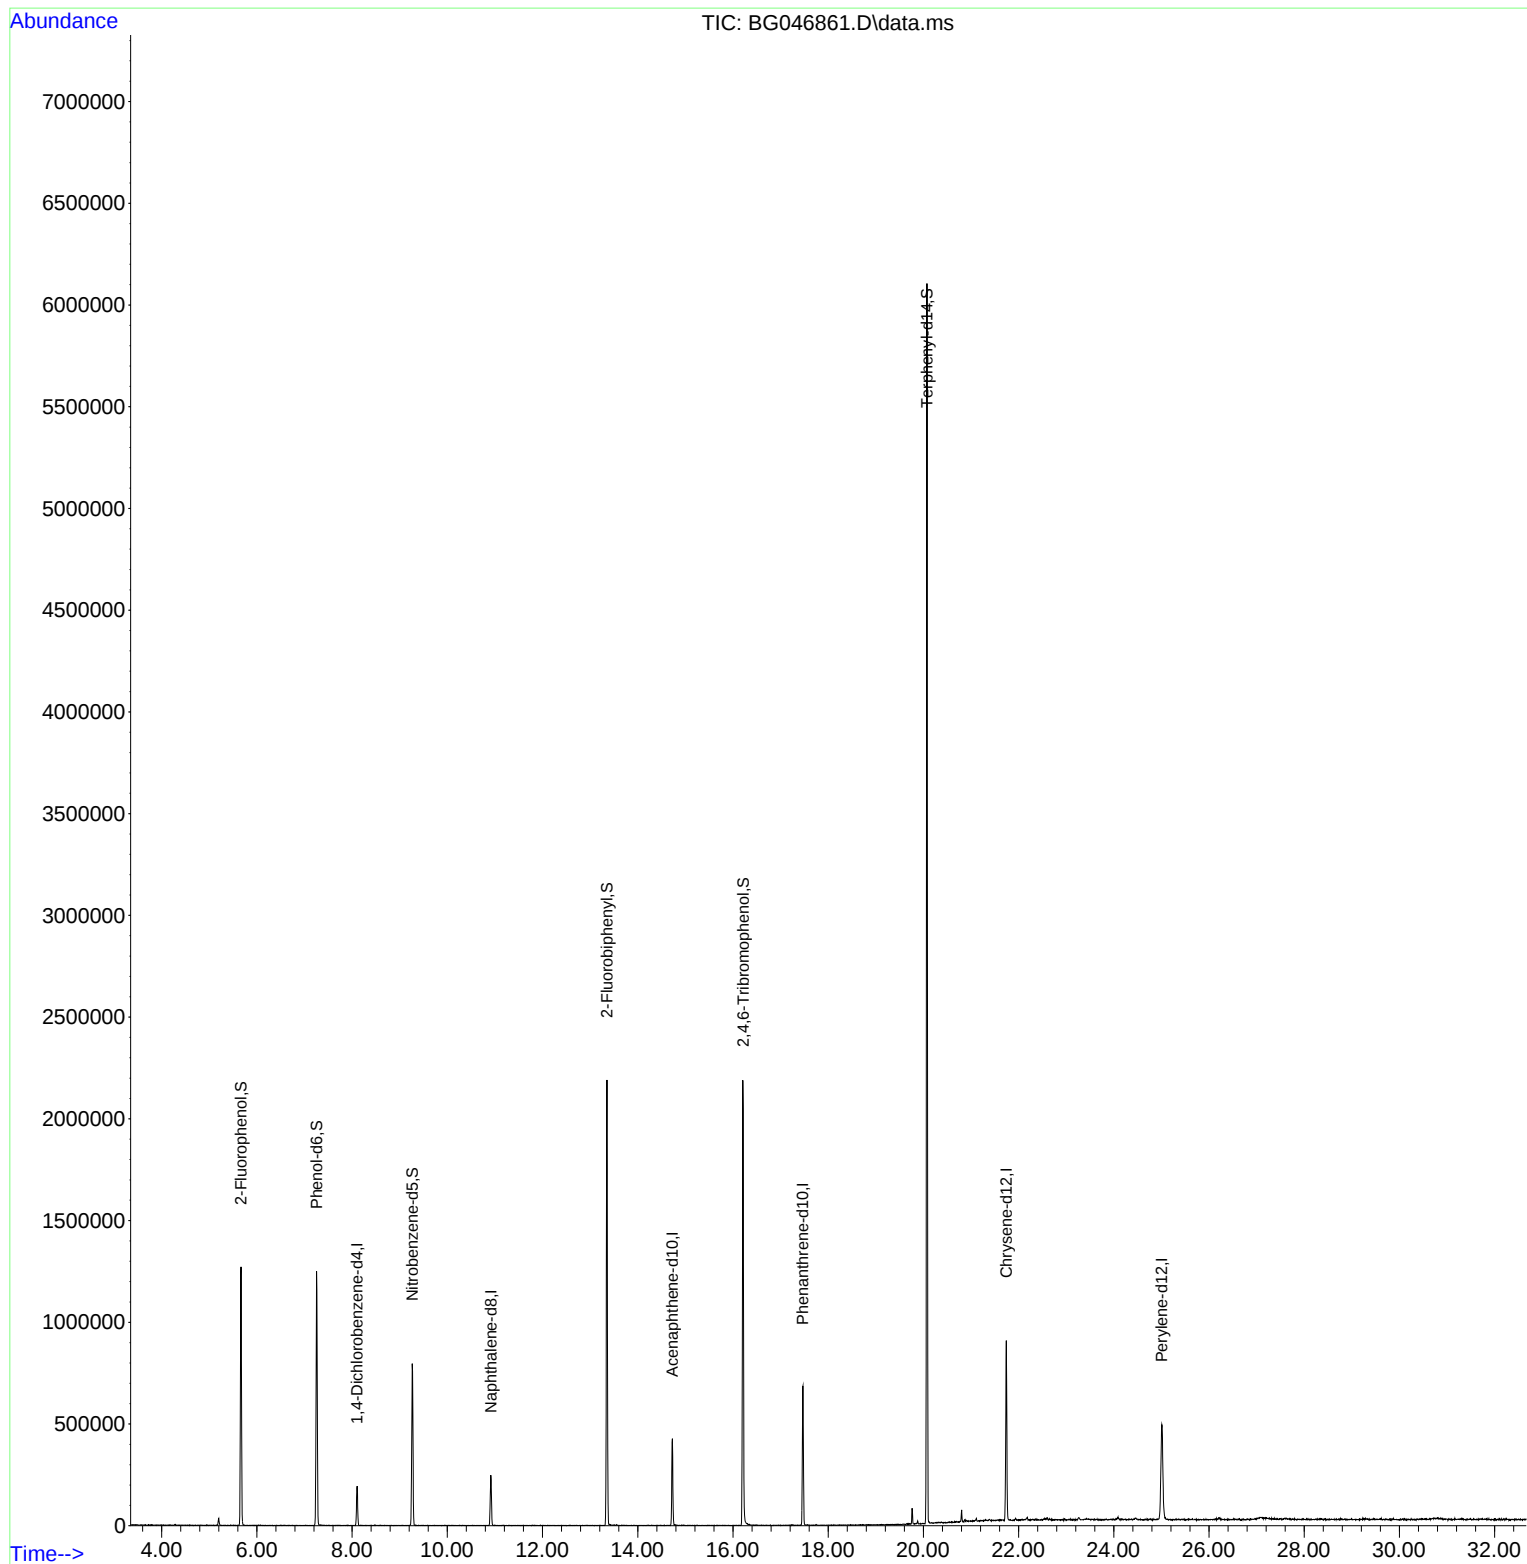




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.106 min Scan# 811
Delta R.T. -0.002 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48




Instrument :
BNA_G
ClientSampleId :
PB132258TB


Tgt Ion:152 Resp: 55124
Ion Ratio Lower Upper
152 100
150 146.3 125.0 187.6
115 62.8 41.8 62.6#

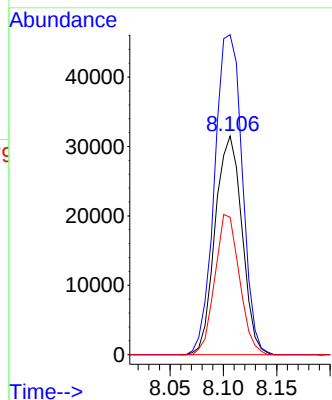

#5
2-Fluorophenol
Concen: 152.56 ng
RT: 5.668 min Scan# 396
Delta R.T. -0.002 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Tgt Ion:112 Resp: 524960
Ion Ratio Lower Upper
112 100
64 63.3 46.7 70.1
63 37.6 22.8 34.2#


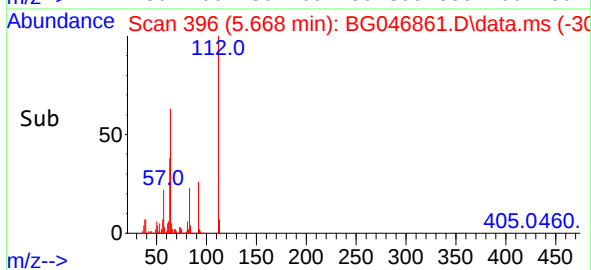
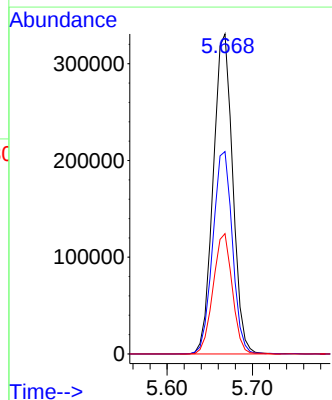





#7
Phenol-d6
Concen: 140.19 ng
RT: 7.254 min Scan# 666
Delta R.T. -0.002 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48




Instrument :
BNA_G
ClientSampleId :
PB132258TB


Tgt Ion: 99 Resp: 680409
Ion Ratio Lower Upper
99 100
42 20.1 12.8 19.2#
71 42.6 24.6 36.8#

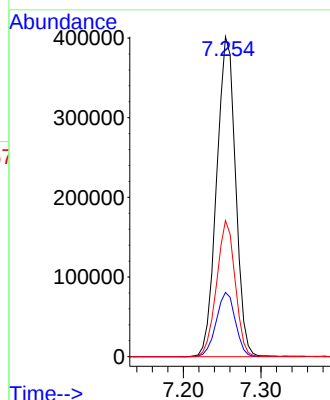

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.915 min Scan# 1289
Delta R.T. -0.008 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Tgt Ion: 136 Resp: 206001
Ion Ratio Lower Upper
136 100
137 9.5 9.1 13.7
54 7.7 6.2 9.4
68 3.9 5.0 7.4#


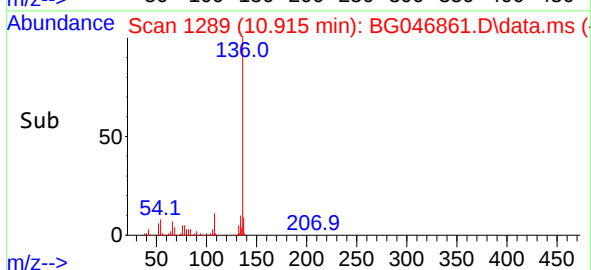
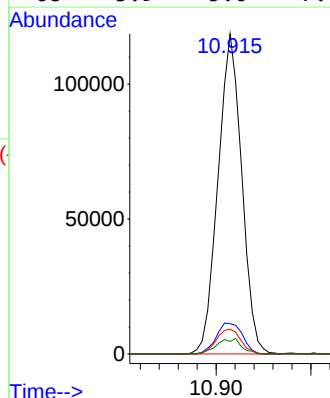



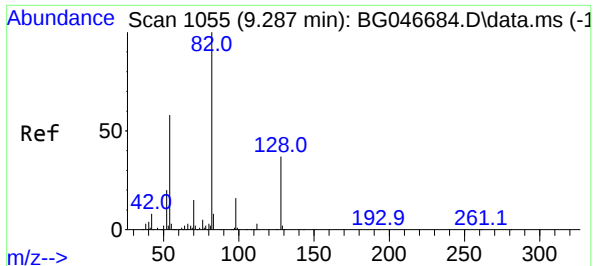

#23
Nitrobenzene-d5
Concen: 123.24 ng
RT: 9.264 min Scan# 1008
Delta R.T. -0.008 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48




Instrument :
BNA_G
ClientSampleId :
PB132258TB


Tgt Ion: 82 Resp: 477217
Ion Ratio Lower Upper
82 100
128 42.1 37.0 55.6
54 53.1 39.0 58.4

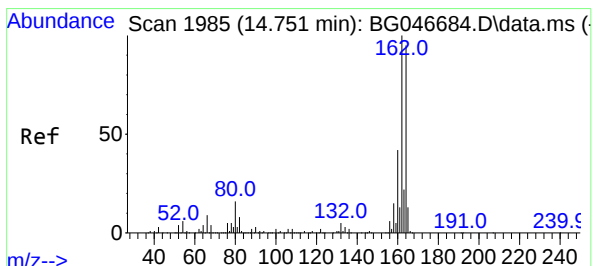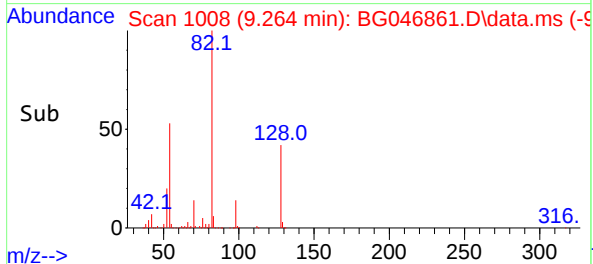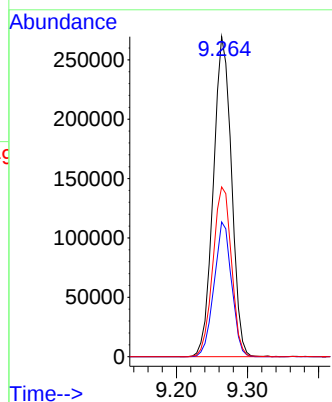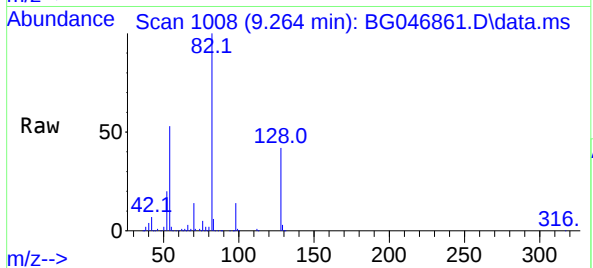

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.728 min Scan# 1938
Delta R.T. -0.008 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48


Tgt Ion:164 Resp: 155429
Ion Ratio Lower Upper
164 100
162 96.3 82.3 123.5
160 41.2 35.3 52.9

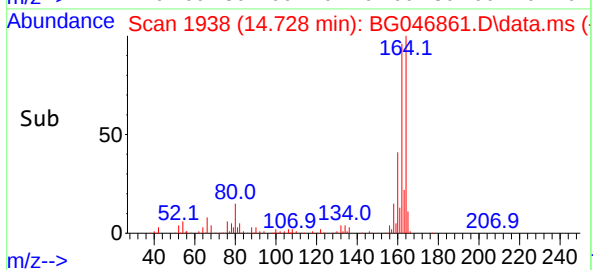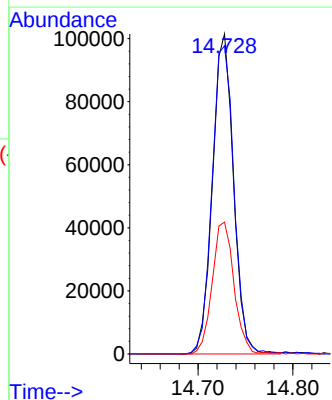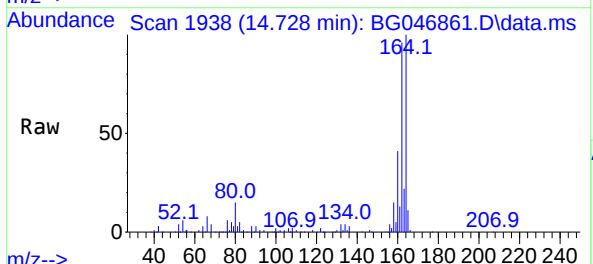






#42
2,4,6-Tribromophenol
Concen: 208.73 ng
RT: 16.214 min Scan# 2191
Delta R.T. -0.002 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48


Instrument :
BNA_G
ClientSampleID :
PB132258TB

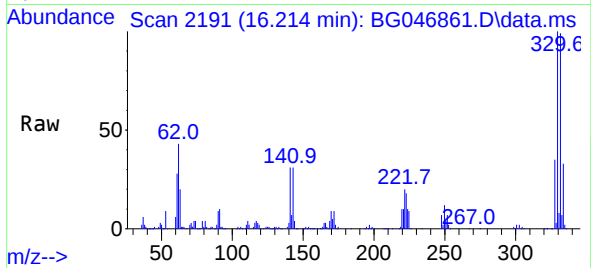



Tgt Ion:330 Resp: 427779
Ion Ratio Lower Upper
330 100
332 97.4 76.5 114.7
141 34.1 26.0 39.0

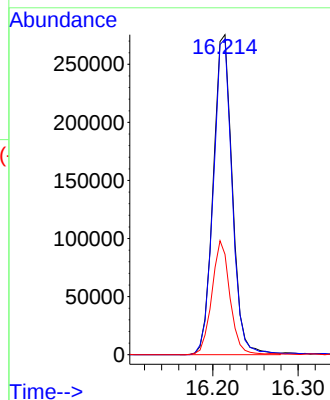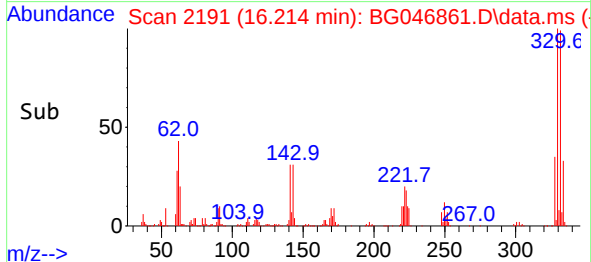


#45
2-Fluorobiphenyl
Concen: 102.18 ng
RT: 13.353 min Scan# 1704
Delta R.T. -0.008 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48




Tgt Ion:172 Resp: 1121826
Ion Ratio Lower Upper
172 100
171 37.0 31.3 46.9
170 24.7 20.8 31.2

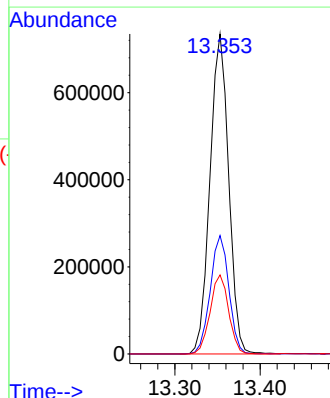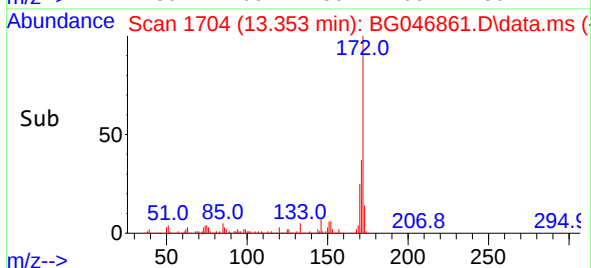






#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.466 min Scan# 2404
Delta R.T. -0.013 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Instrument :
BNA_G
ClientSampleId :
PB132258TB



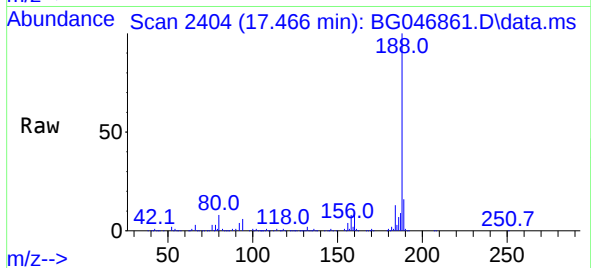



Tgt Ion:188 Resp: 456602
Ion Ratio Lower Upper
188 100
94 5.9 6.3 9.5#
80 8.1 7.0 10.6

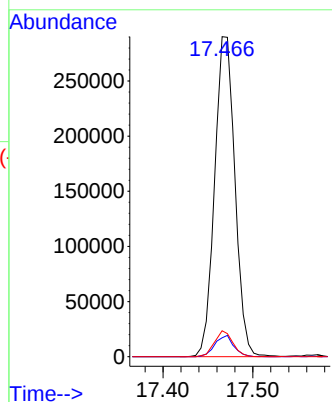

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.743 min Scan# 3132
Delta R.T. -0.013 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Tgt Ion:240 Resp: 551070
Ion Ratio Lower Upper
240 100
120 5.6 6.2 9.4#
236 26.2 20.5 30.7


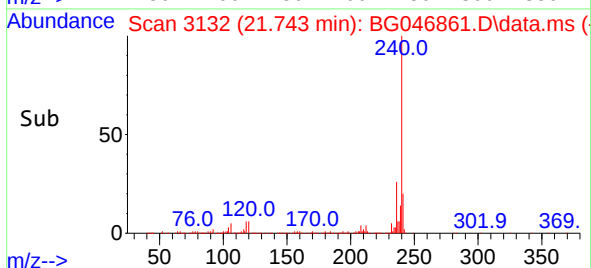
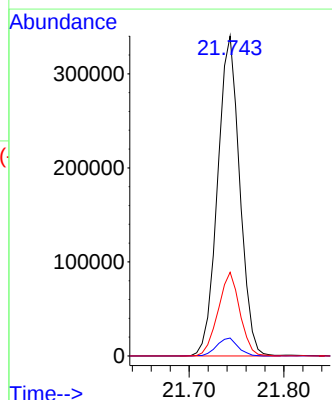





#79
Terphenyl-d14
Concen: 95.00 ng
RT: 20.074 min Scan# 2848
Delta R.T. -0.008 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Instrument :
BNA_G
ClientSampleId :
PB132258TB

Tgt Ion:244 Resp: 2612189
Ion Ratio Lower Upper
244 100
212 9.2 6.7 10.1
122 8.3 7.8 11.6

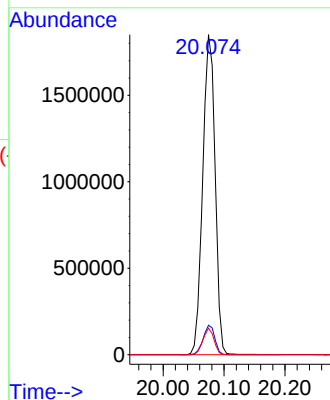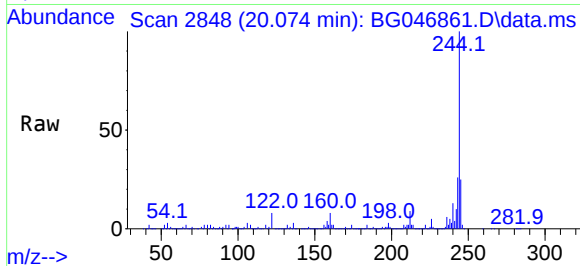

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.010 min Scan# 3688
Delta R.T. -0.019 min
Lab File: BG046861.D
Acq: 13 Oct 2020 3:48

Tgt Ion:264 Resp: 536257
Ion Ratio Lower Upper
264 100
260 24.6 18.8 28.2
265 22.3 17.8 26.8

