
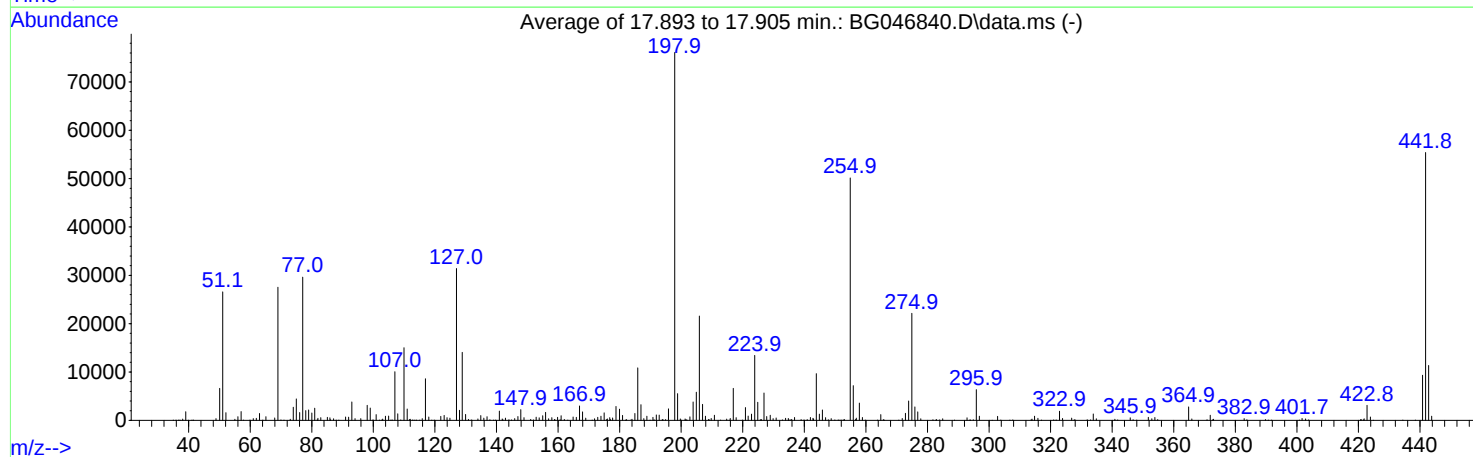


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
Data File : BG046840.D
Acq On : 12 Oct 2020 8:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

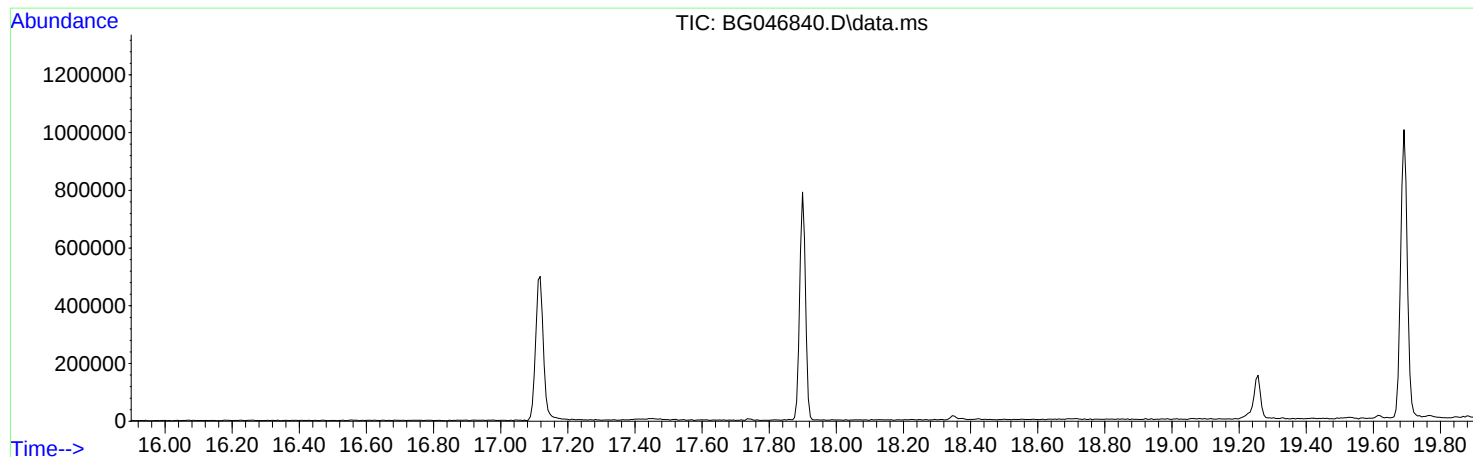

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	26576	PASS
68	69	0.00	2	1.8	491	PASS
69	198	0.00	100	36.2	27533	PASS
70	69	0.00	2	0.4	97	PASS
127	198	10	80	41.3	31403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76085	PASS
199	198	5	9	7.3	5522	PASS
275	198	10	60	29.1	22136	PASS
365	198	1	100	3.7	2794	PASS
441	198	0.01	100	12.3	9340	PASS
442	198	50	100	72.8	55405	PASS
443	442	15	24	20.5	11362	PASS