
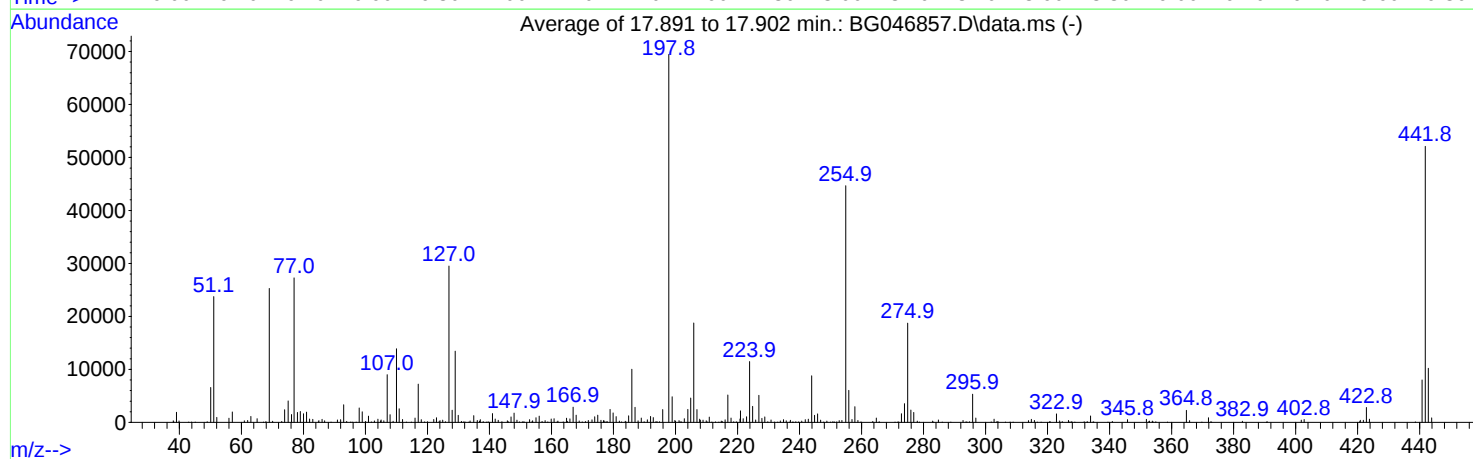


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101220\
 Data File : BG046857.D
 Acq On : 12 Oct 2020 23:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 11:38:17 2020

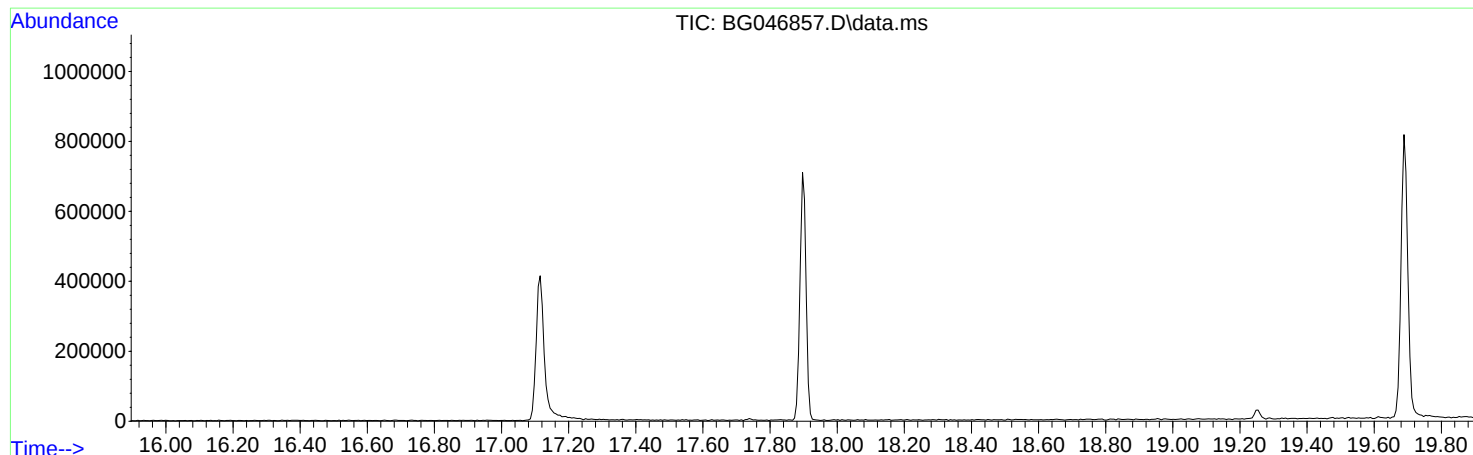

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	23749	PASS
68	69	0.00	2	0.6	142	PASS
69	198	0.00	100	36.4	25272	PASS
70	69	0.00	2	0.9	220	PASS
127	198	10	80	42.5	29499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69435	PASS
199	198	5	9	7.0	4848	PASS
275	198	10	60	27.0	18713	PASS
365	198	1	100	3.3	2277	PASS
441	198	0.01	100	11.5	8011	PASS
442	198	50	100	75.0	52101	PASS
443	442	15	24	19.6	10205	PASS