
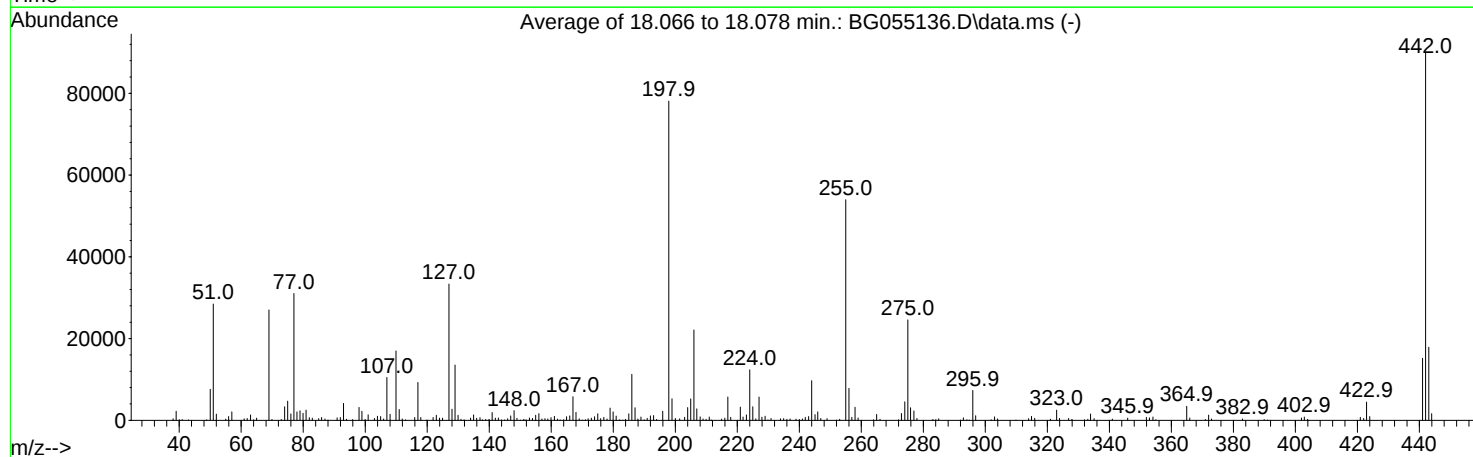


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101222\  
 Data File : BG055136.D  
 Acq On : 12 Oct 2022 10:18  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100322.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Oct 08 03:04:59 2022

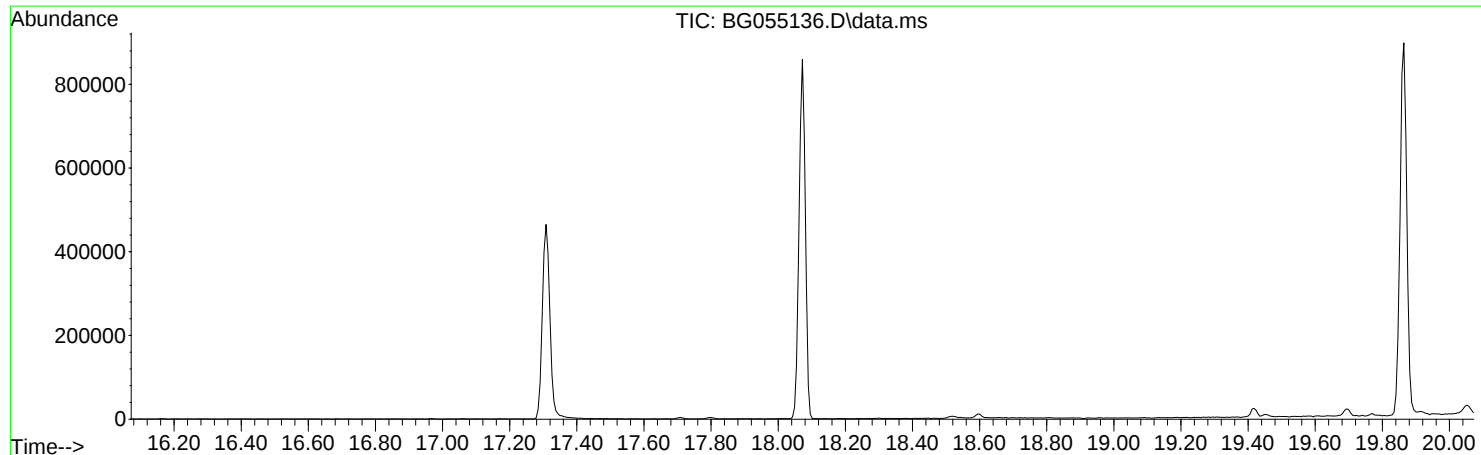




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.4         | 28440      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 34.6         | 27004      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 214        | PASS                |
| 127            | 198             | 10              | 80              | 42.7         | 33333      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 78096      | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 5275       | PASS                |
| 275            | 198             | 10              | 60              | 31.5         | 24584      | PASS                |
| 365            | 198             | 1               | 100             | 4.4          | 3442       | PASS                |
| 441            | 198             | 0.01            | 100             | 19.4         | 15186      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 90011      | PASS                |
| 443            | 442             | 15              | 24              | 19.8         | 17862      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101222\  
Data File : BG055136.D  
Acq On : 12 Oct 2022 10:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 13 05:30:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 08 03:04:59 2022  
Response via : Initial Calibration

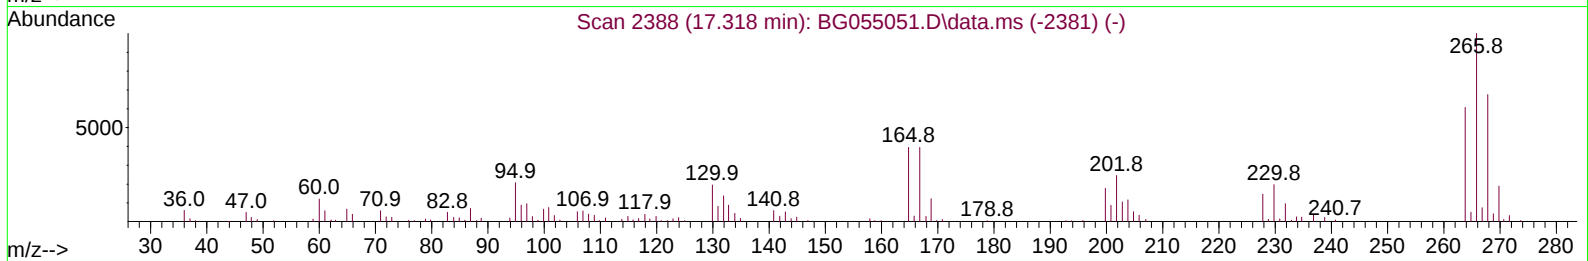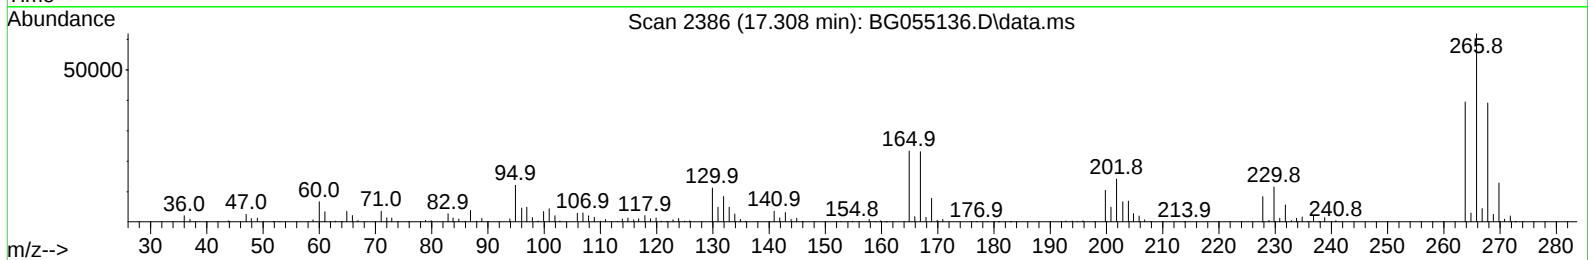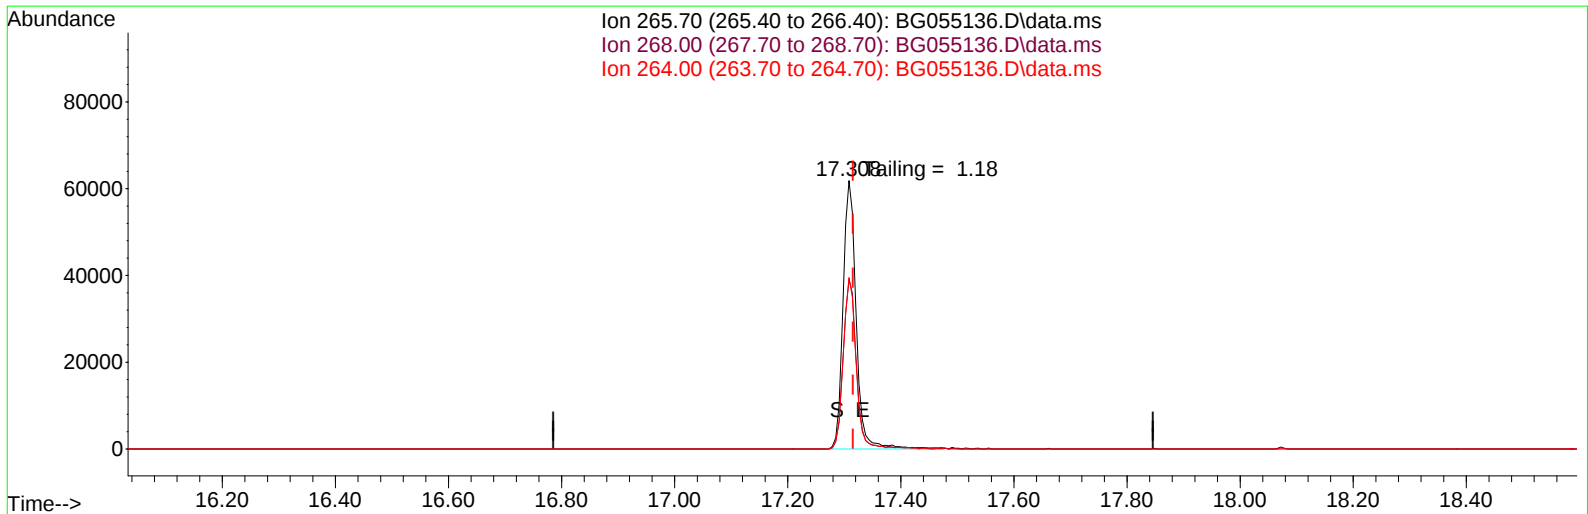

TIC: BG055136.D\data.ms

**(70) Pentachlorophenol (C)**

17.308min (-0.007) 85957.05 ng




response 99833

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 67.50  | 63.20  |
| 264.00 | 60.80  | 63.88  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG101222\  
Data File : BG055136.D  
Acq On : 12 Oct 2022 10:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Oct 13 05:30:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100322.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Oct 08 03:04:59 2022  
Response via : Initial Calibration

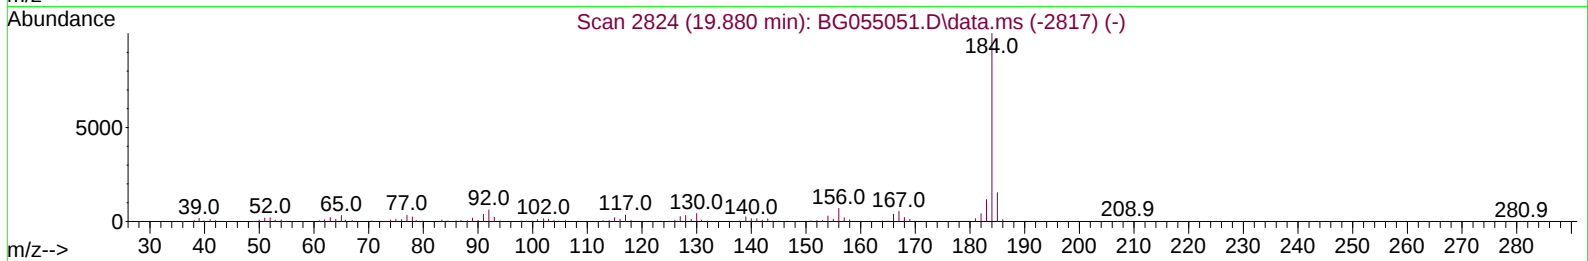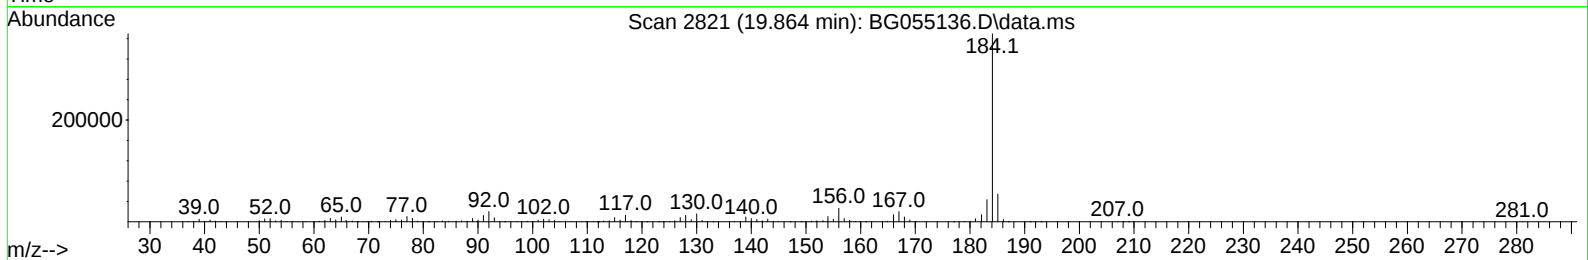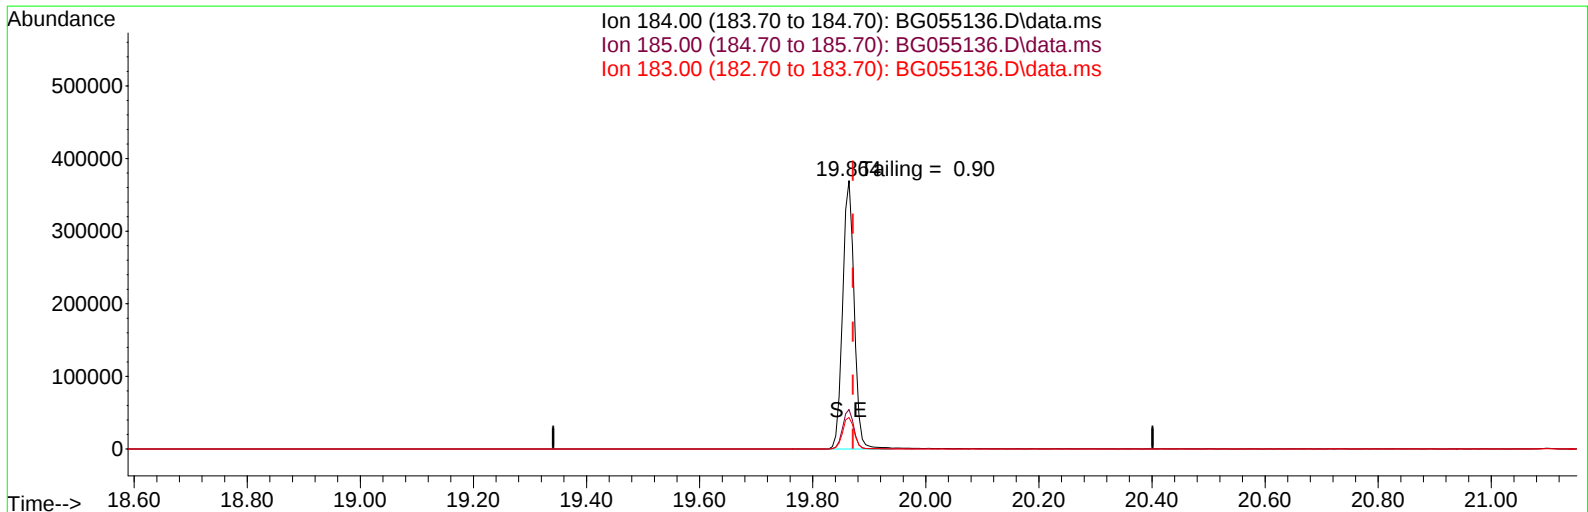

TIC: BG055136.D\data.ms

(77) Benzidine

19.864min (-0.007) 14848.65 ng

response 524133

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.30  | 14.75  |
| 183.00 | 11.70  | 11.74  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 10/12/2022    | BNA_G            | <u>BG055136.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 237817           | 21.098             |
| DDD           | 8787             | 20.646             |
| DDE           | 325              | 20.152             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 9112          | 246929           | 3.69               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP