
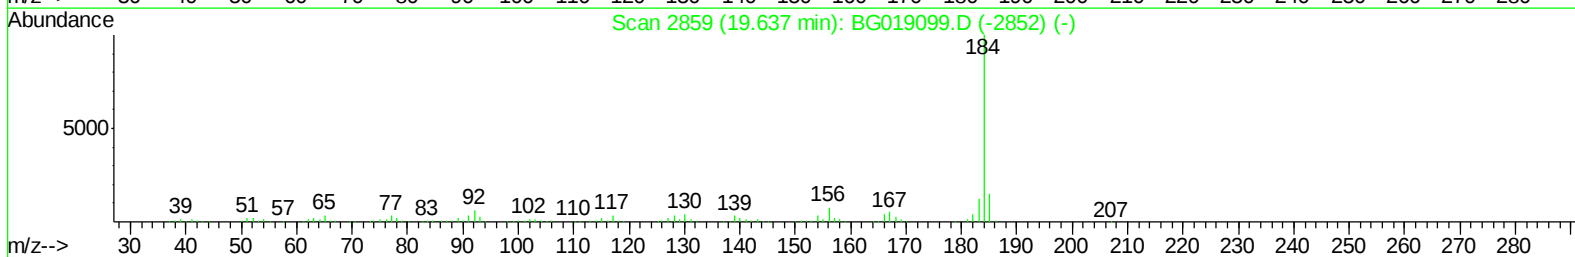
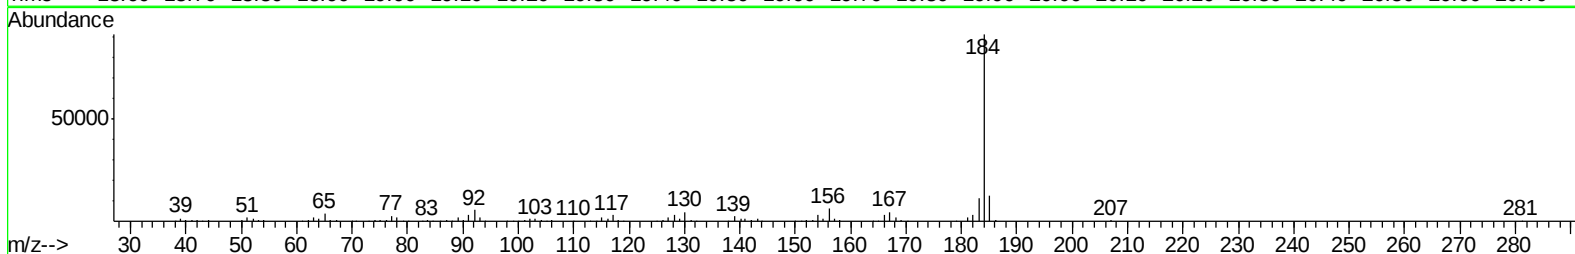


Data Path : Z:\HPCHEM1\BNA G\Data\BG101315\
Data File : BG019164.D
Acq On : 12 Oct 2015 19:10
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 03:38:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 10 07:04:31 2015
Response via : Initial Calibration

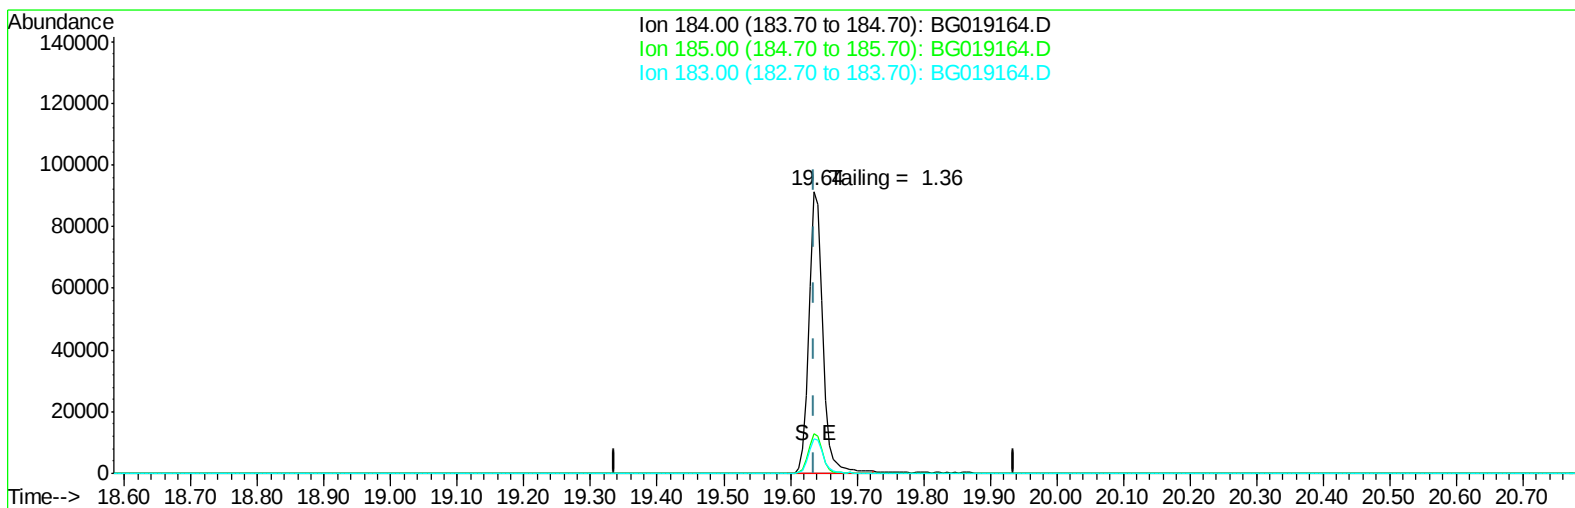

TIC: BG019164.D

(76) Benzidine




19.636min (-0.001) 0.00ng

response 135669

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	14.20
183.00	12.60	12.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG101315\
Data File : BG019164.D
Acq On : 12 Oct 2015 19:10
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 03:38:31 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 10 07:04:31 2015
Response via : Initial Calibration

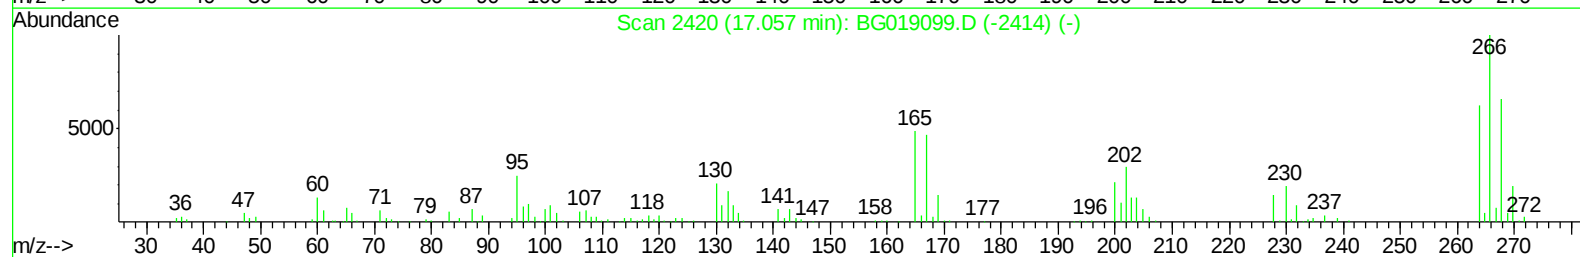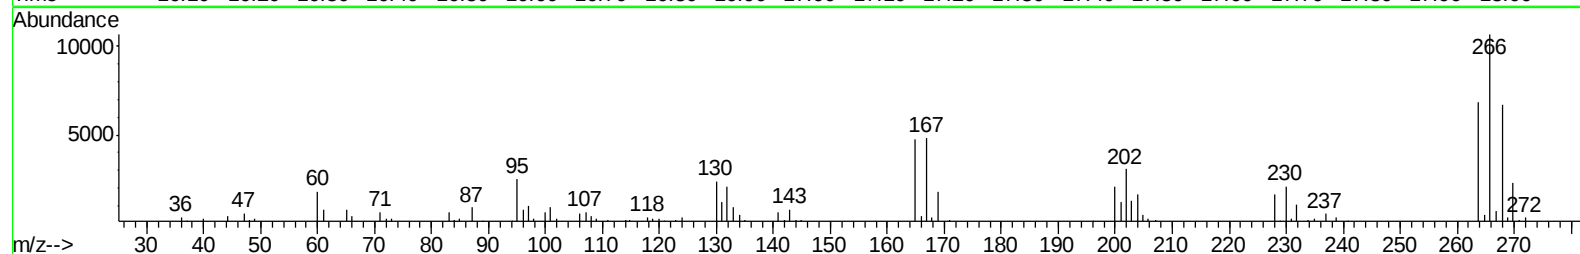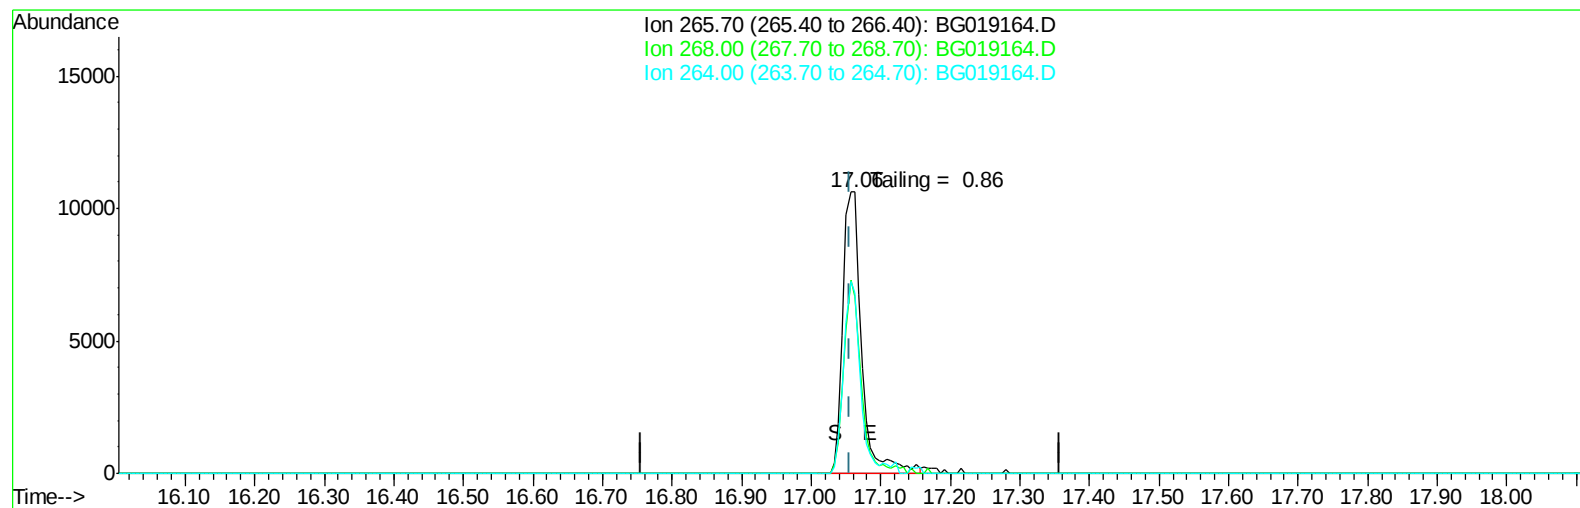

TIC: BG019164.D

(69) Pentachlorophenol (C)

17.062min (+0.005) 0.00ng

response 18934

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	62.91
264.00	62.60	64.05
0.00	0.00	0.00