


Data Path : Z:\HPCHEM1\BNA G\Data\BG101315\
 Data File : BG019164.D
 Acq On : 12 Oct 2015 19:10
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 10 07:04:31 2015

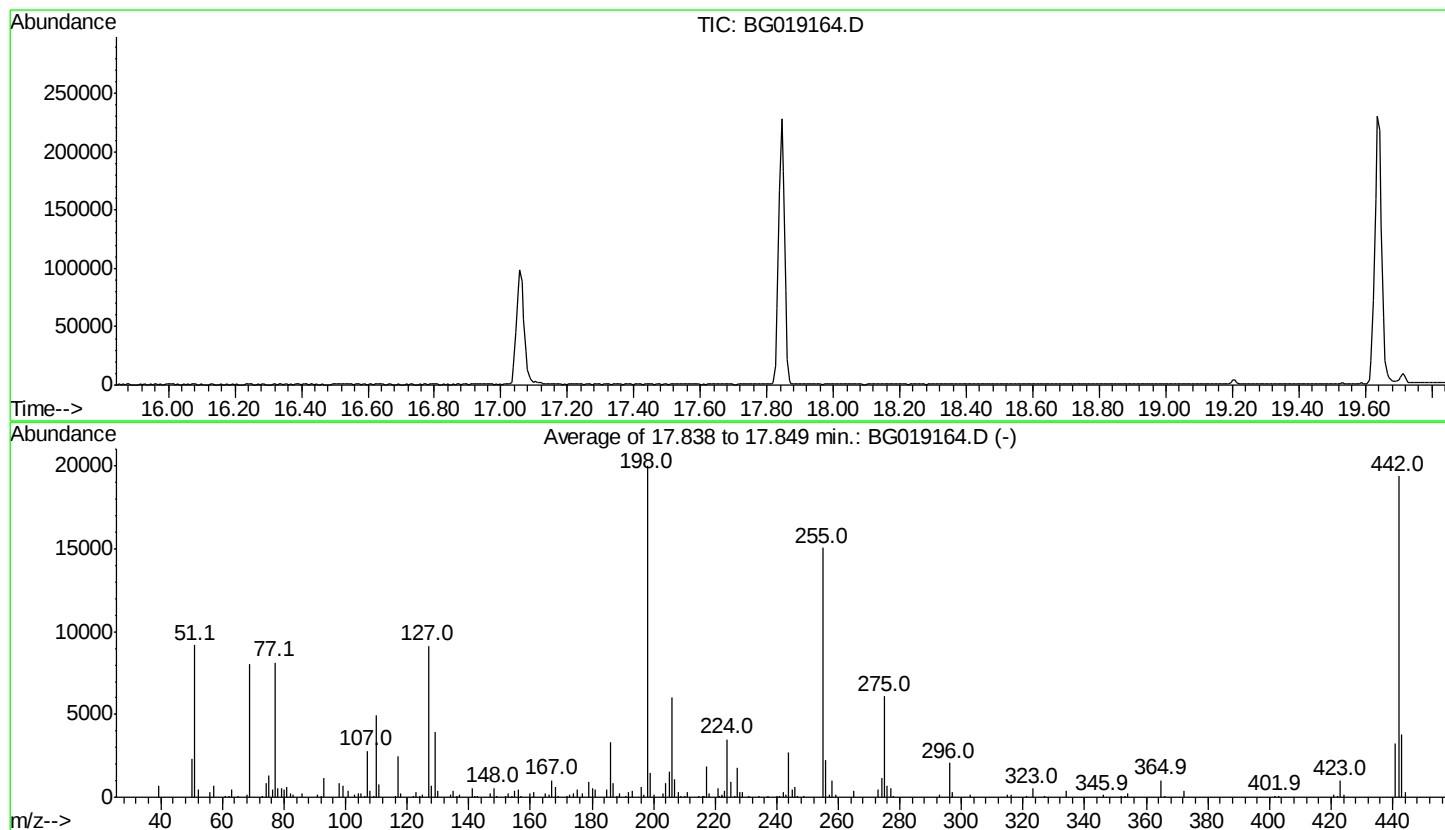

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	9197	PASS
68	69	0.00	2	1.9	153	PASS
69	198	0.00	100	40.1	8033	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.6	9141	PASS
197	198	0.00	2	0.7	143	PASS
198	198	100	100	100.0	20032	PASS
199	198	5	9	7.2	1434	PASS
275	198	10	60	30.4	6095	PASS
365	198	1	100	5.1	1014	PASS
441	442	0.01	24	16.6	3217	PASS
442	198	50	100	96.8	19394	PASS
443	442	15	24	19.5	3785	PASS