

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024320.D
 Acq On : 13 Oct 2016 14:43
 Operator : UM/SJ
 Sample : H5166-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNJ2

Quant Time: Oct 13 16:06:27 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 13 01:34:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	221606	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	951663	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	708836	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1306518	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1483288	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1545280	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	13860	2.97	ng/uL	0.00
5) Phenol-d5	7.42	99	376675	18.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	249070	17.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	262451	18.43	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	309547	18.52	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	136990	20.28	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	155506	20.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	304064	18.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	323189	18.69	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	970498	19.61	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1122634	19.80	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	152276	17.35	ng/ul	0.00
57) Fluorene-d10	15.89	176	885030	18.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	164147	20.91	ng/ul	0.00
70) Anthracene-d10	17.74	188	1280008	21.69	ng/ul	0.00
76) Pyrene-d10	20.01	212	1519116	21.94	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	1536761	22.10	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.34	163	560109	11.54	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024320.D
Acq On : 13 Oct 2016 14:43
Operator : UM/SJ
Sample : H5166-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNJ2

Quant Time: Oct 13 16:06:27 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 13 01:34:23 2016
Response via : Initial Calibration

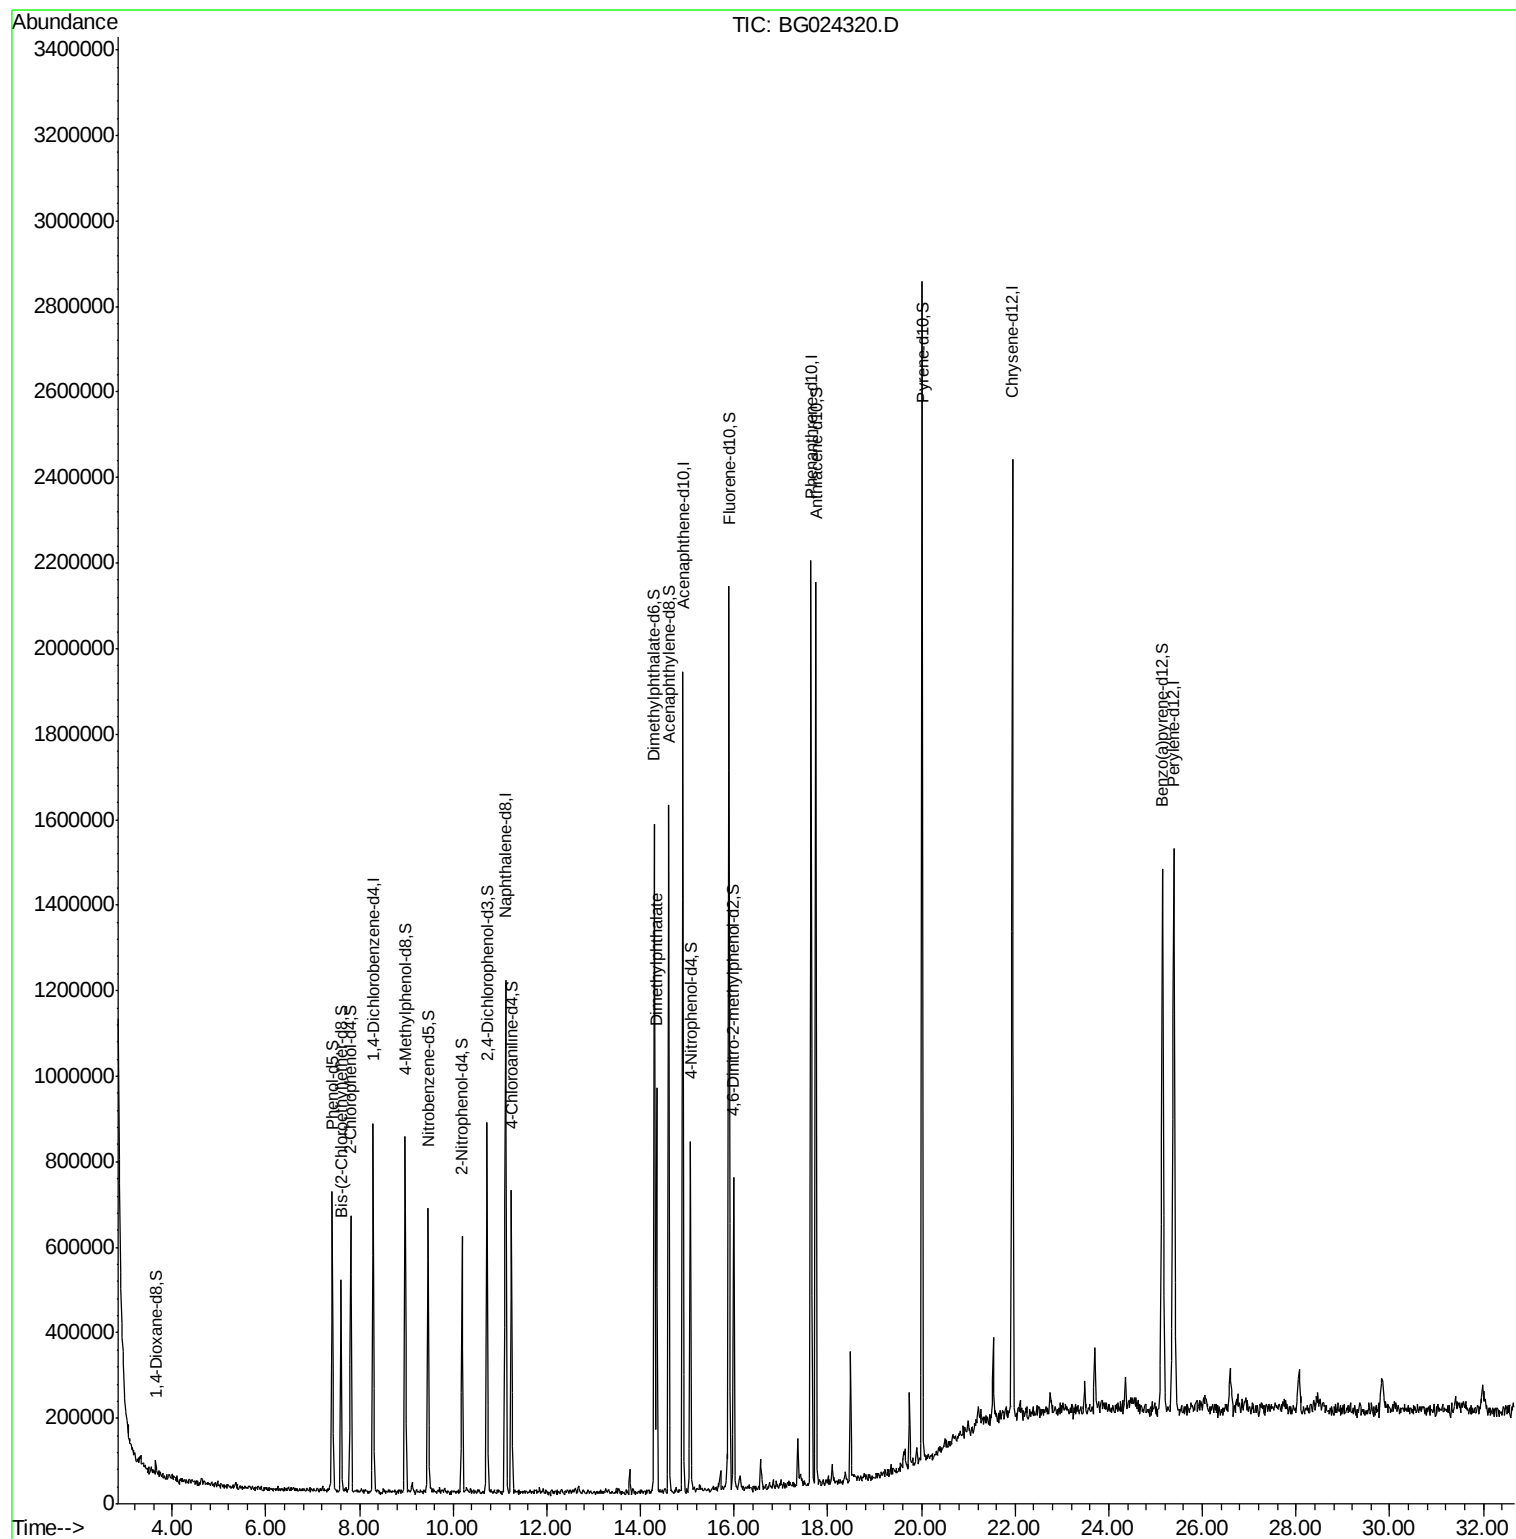

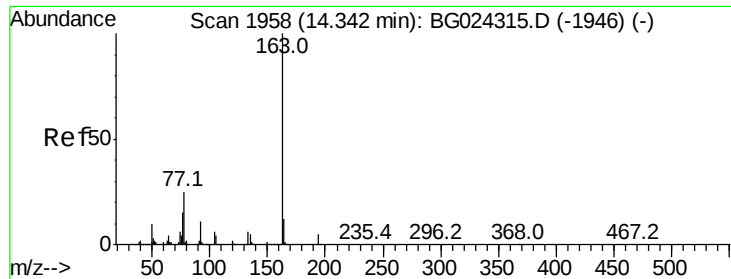

#44

Dimethylphthalate

Concen: 11.54 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. -0.00 min

Lab File: BG024320.D

Acq: 13 Oct 2016 14:43

Instrument :

BNA_G

ClientSampleId :

BDNJ2

Tot Ion:163 Resp: 560109

Ion Ratio Lower Upper

163 100

194 5.2 3.4 5.0#

164 10.6 9.0 13.4

