

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024326.D
 Acq On : 13 Oct 2016 18:34
 Operator : UM/SJ
 Sample : H5164-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNM5

Quant Time: Oct 14 02:32:14 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	230068	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	997389	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	770700	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1462369	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1650010	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1724605	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	14799	3.05	ng/uL	0.00
5) Phenol-d5	7.42	99	380370	17.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	260435	17.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	269458	18.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	276180	15.92	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	149013	21.05	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	165466	20.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	309733	17.96	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	264536	14.60	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1008412	18.74	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1238460	20.09	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	152092	15.94	ng/ul	0.00
57) Fluorene-d10	15.89	176	983057	19.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	160131	18.22	ng/ul	0.00
70) Anthracene-d10	17.74	188	1378016	20.86	ng/ul	0.00
76) Pyrene-d10	20.01	212	1577652	20.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	1557385	20.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.34	163	826413	15.66	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024326.D
Acq On : 13 Oct 2016 18:34
Operator : UM/SJ
Sample : H5164-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNM5

Quant Time: Oct 14 02:32:14 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

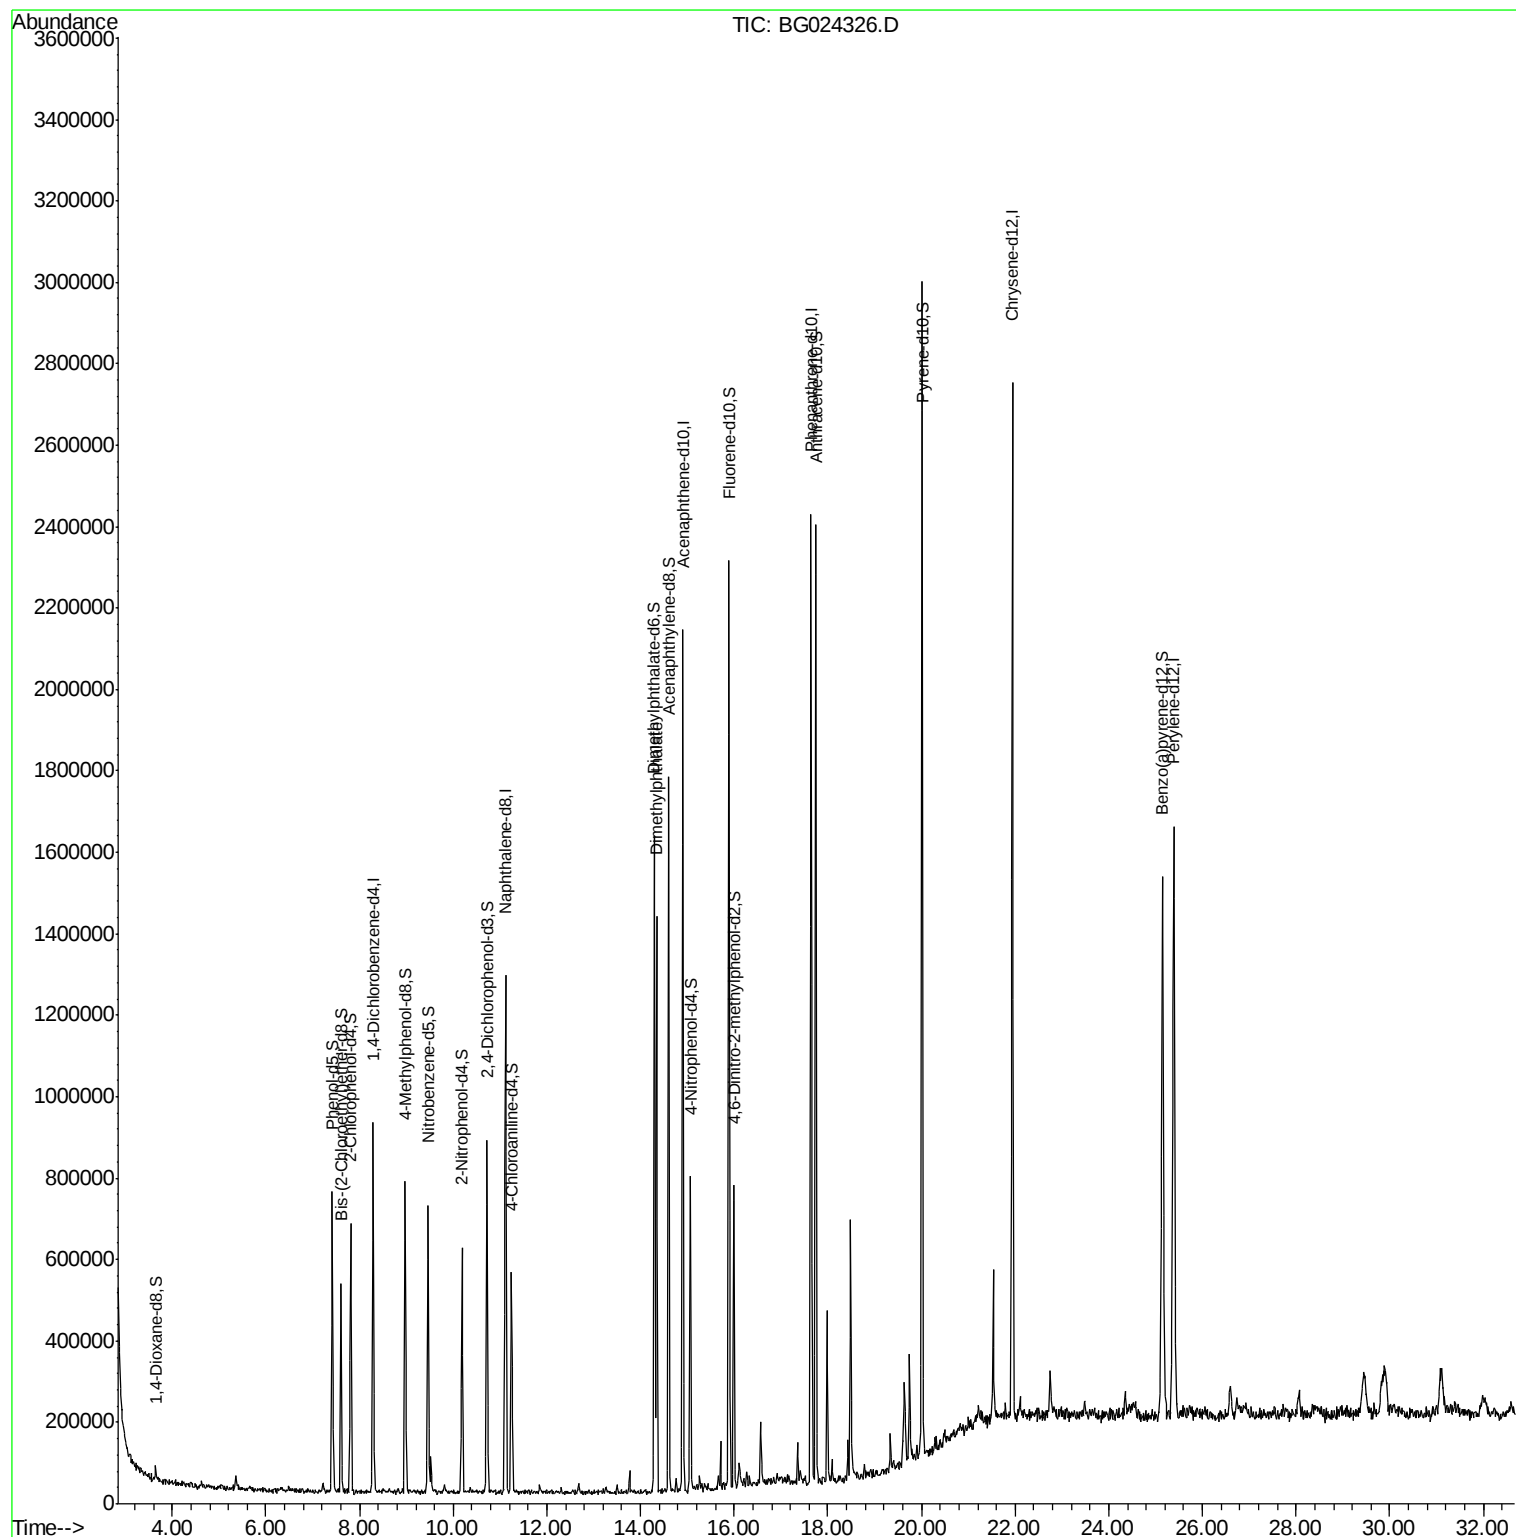

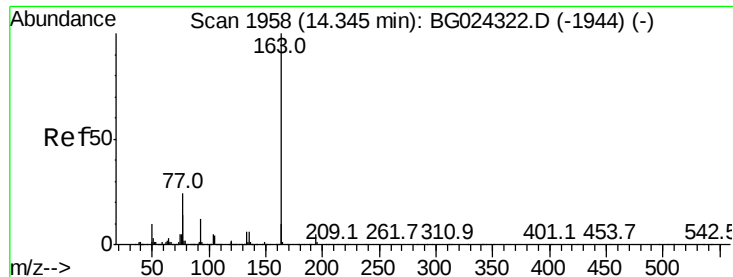

#44

Dimethylphthalate

Concen: 15.66 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. 0.00 min

Lab File: BG024326.D

Acq: 13 Oct 2016 18:34

Instrument :

BNA_G

ClientSampleId :

BDNM5


Tot Ion:163 Resp: 826413

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 10.8 9.0 13.4

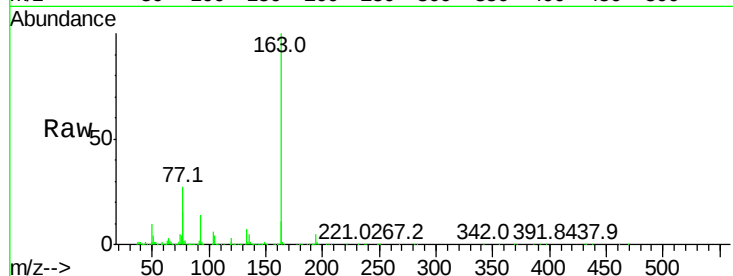

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

