

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024330.D
 Acq On : 13 Oct 2016 21:08
 Operator : UM/SJ
 Sample : H5166-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNK4

Quant Time: Oct 14 02:32:53 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	194631	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	868871	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	690709	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1289780	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1476322	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1505514	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	24330	5.94	ng/uL	0.00
5) Phenol-d5	7.42	99	548838	30.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	369374	30.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	384967	30.79	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	461551	31.44	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	194574	31.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	241293	34.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	446586	29.72	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	568649	36.02	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1371940	28.45	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1618792	29.30	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	214761	25.11	ng/ul	0.00
57) Fluorene-d10	15.89	176	1258651	27.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	232351	29.98	ng/ul	0.00
70) Anthracene-d10	17.74	188	1759662	30.20	ng/ul	0.00
76) Pyrene-d10	20.01	212	1999214	29.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	2120241	31.30	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.34	163	676112	14.30	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024330.D
Acq On : 13 Oct 2016 21:08
Operator : UM/SJ
Sample : H5166-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNK4

Quant Time: Oct 14 02:32:53 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

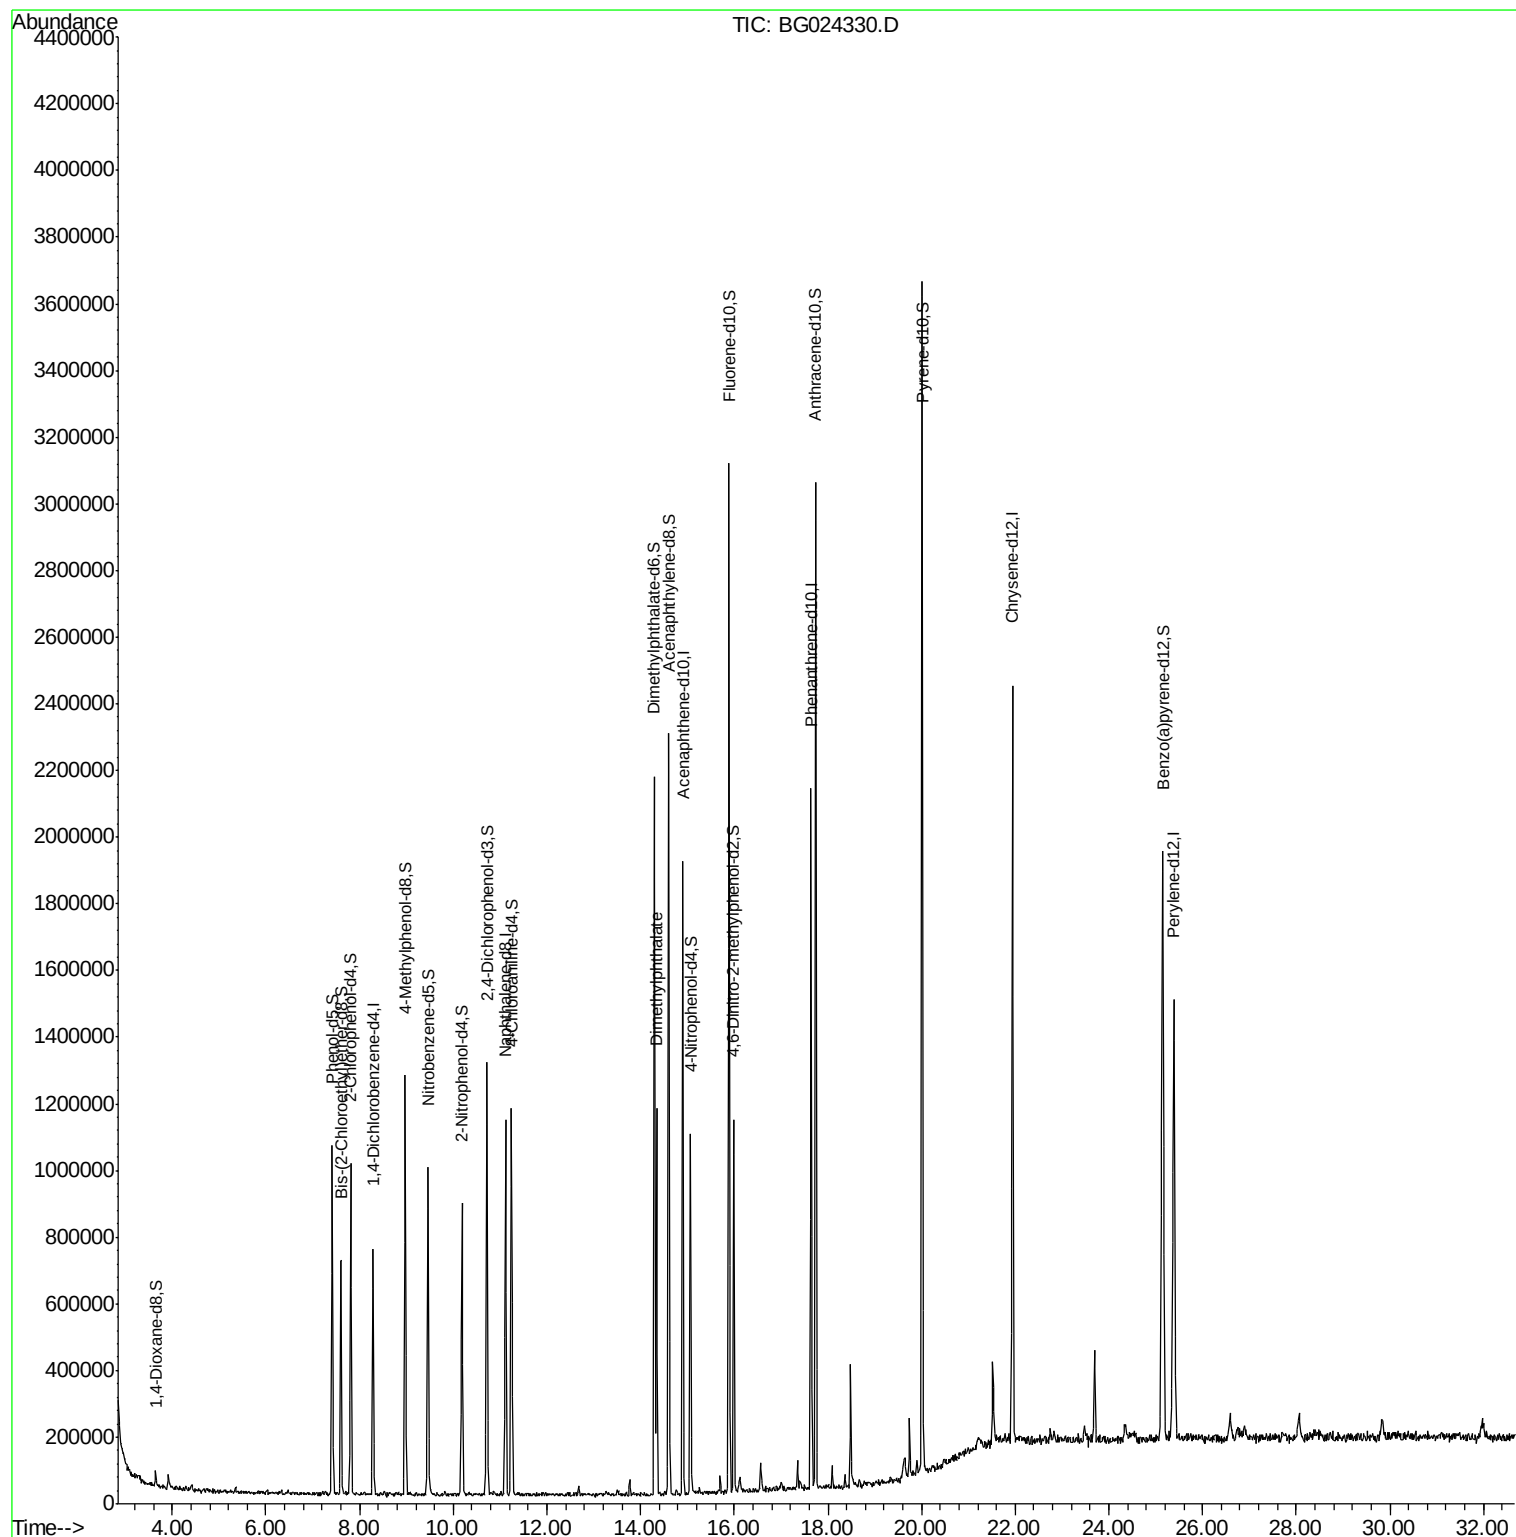

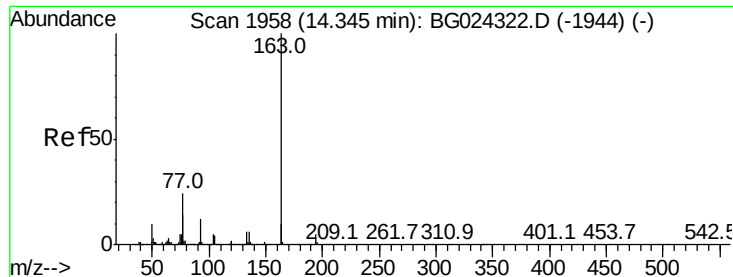

#44

Dimethylphthalate

Concen: 14.30 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. 0.00 min

Lab File: BG024330.D

Acq: 13 Oct 2016 21:08

Instrument :

BNA_G

ClientSampleId :

BDNK4


Tot Ion:163 Resp: 676112

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.1 9.0 13.4

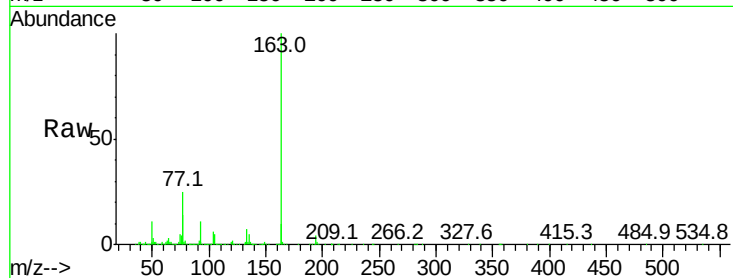

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

