

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024331.D
 Acq On : 13 Oct 2016 21:46
 Operator : UM/SJ
 Sample : H5166-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNK5

Quant Time: Oct 14 02:33:02 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	225298	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	975702	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	746909	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1390877	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1614406	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1687409	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	12727	2.68	ng/uL	0.00
5) Phenol-d5	7.41	99	370954	17.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	239761	16.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	256803	17.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	296739	17.46	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	137578	19.87	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	158092	20.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	303914	18.01	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	364146	20.54	ng/ul	0.00
43) Dimethylphthalate-d6	14.29	166	987149	18.93	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1161446	19.44	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	148894	16.10	ng/ul	0.00
57) Fluorene-d10	15.89	176	900400	18.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	156702	18.75	ng/ul	0.00
70) Anthracene-d10	17.74	188	1254508	19.97	ng/ul	0.00
76) Pyrene-d10	20.01	212	1497650	19.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	1566209	20.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.34	163	725533	14.19	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024331.D
Acq On : 13 Oct 2016 21:46
Operator : UM/SJ
Sample : H5166-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNK5

Quant Time: Oct 14 02:33:02 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

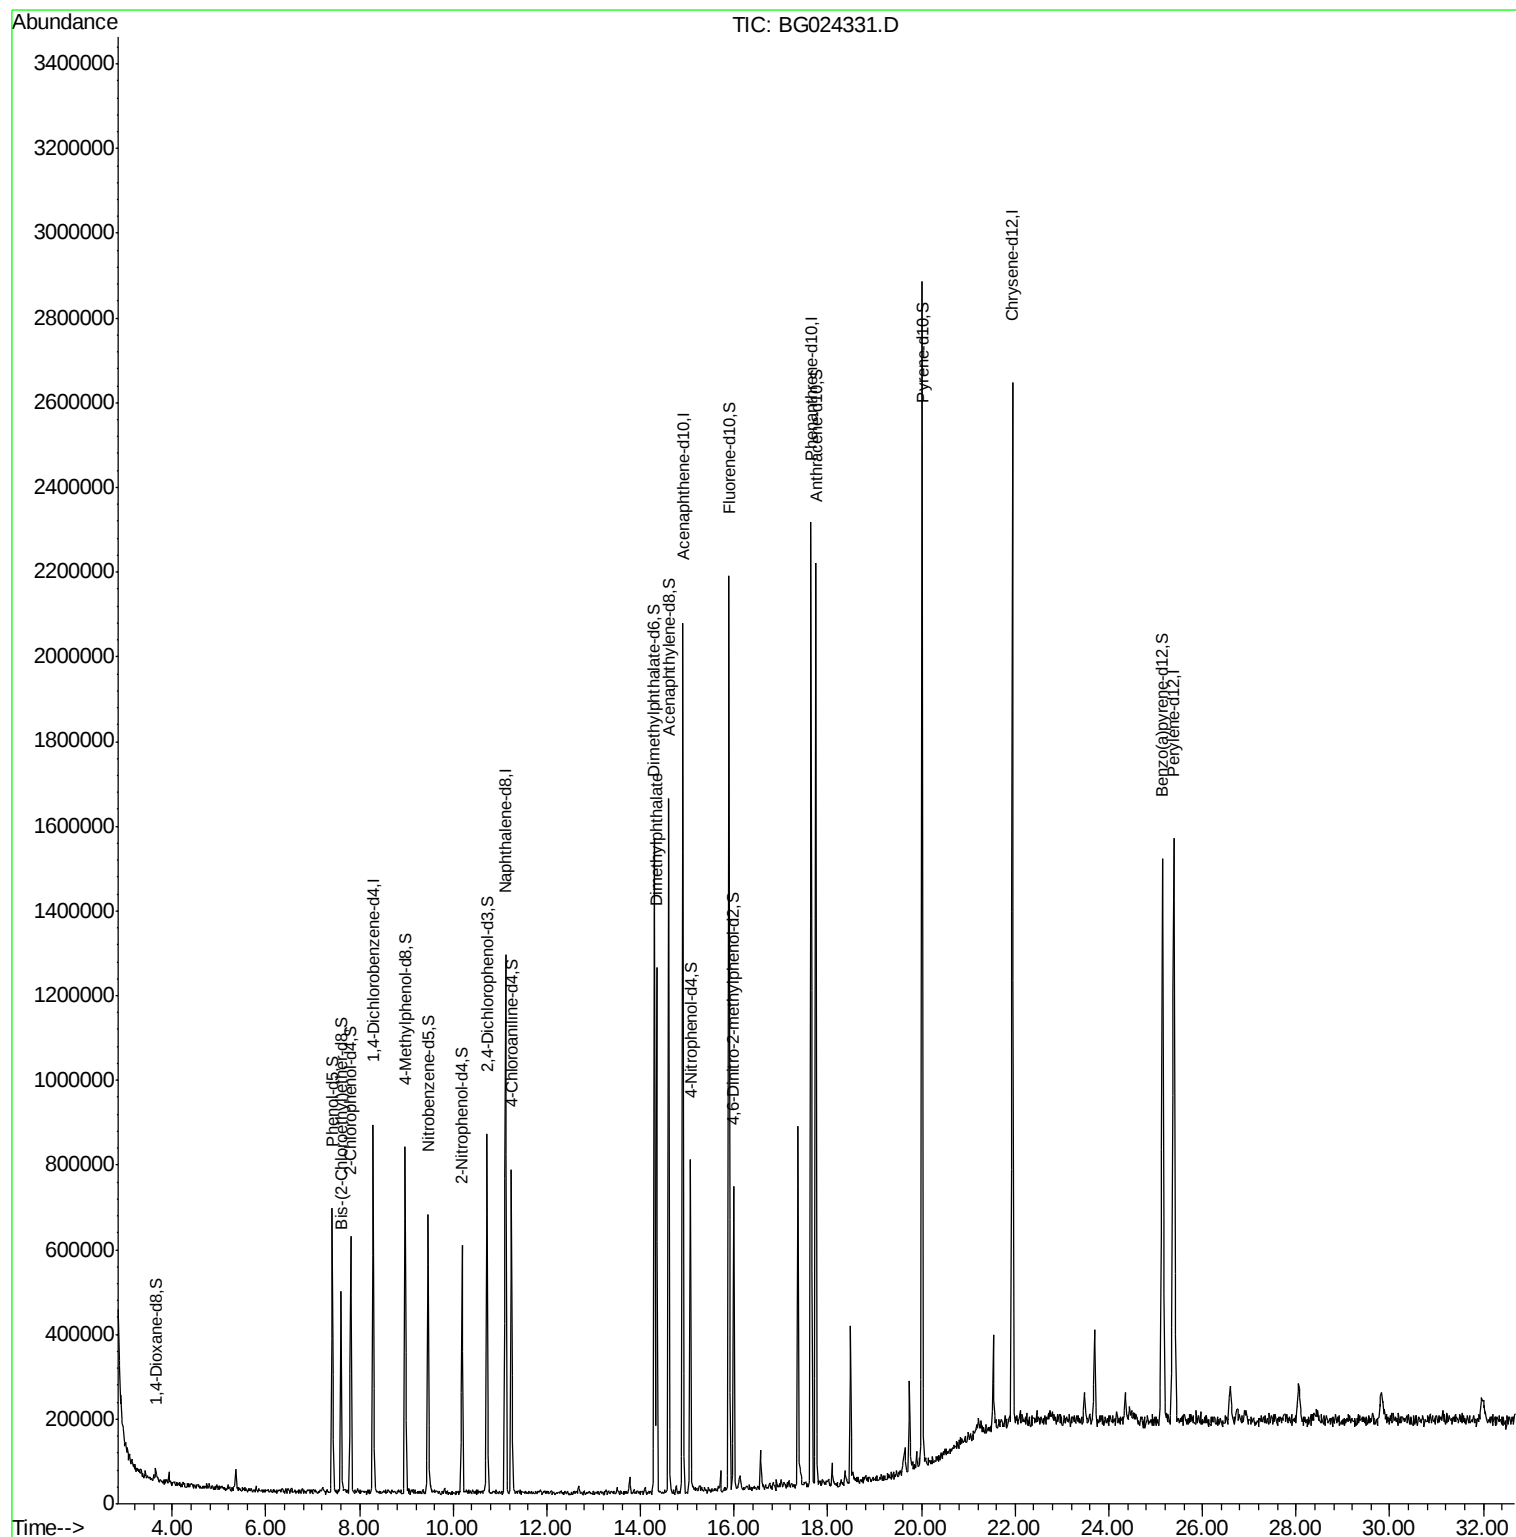

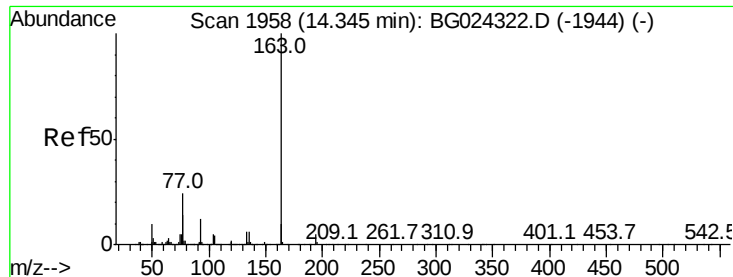

#44

Dimethylphthalate

Concen: 14.19 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. -0.00 min

Lab File: BG024331.D

Acq: 13 Oct 2016 21:46

Instrument :

BNA_G

ClientSampleId :

BDNK5


Tot Ion:163 Resp: 725533

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 10.1 9.0 13.4

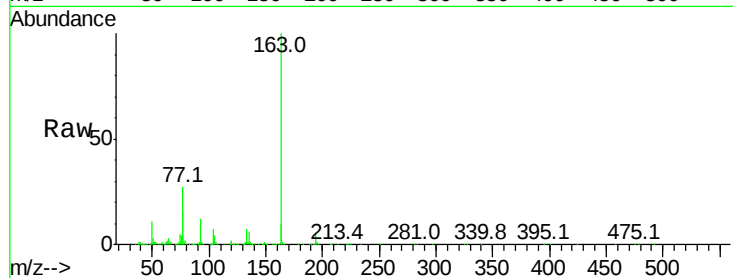

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

