

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024332.D
 Acq On : 13 Oct 2016 22:25
 Operator : UM/SJ
 Sample : H5166-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNH9

Quant Time: Oct 14 02:33:11 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	212996	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	936192	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	690573	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1319931	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1464667	20.00	ng/ul	0.00
83) Perylene-d12	25.38	264	1516667	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	16646	3.71	ng/uL	0.00
5) Phenol-d5	7.42	99	415880	20.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	281264	20.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	302758	22.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	337469	21.01	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	153628	23.12	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	184364	24.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	336662	20.80	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	422820	24.86	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1081476	22.43	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1276525	23.11	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	176588	20.65	ng/ul	0.00
57) Fluorene-d10	15.89	176	985892	21.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	175899	22.17	ng/ul	0.00
70) Anthracene-d10	17.74	188	1370326	22.98	ng/ul	0.00
76) Pyrene-d10	20.01	212	1583196	23.16	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.14	264	1606986	23.55	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.34	163	791187	16.73	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024332.D
Acq On : 13 Oct 2016 22:25
Operator : UM/SJ
Sample : H5166-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNH9

Quant Time: Oct 14 02:33:11 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

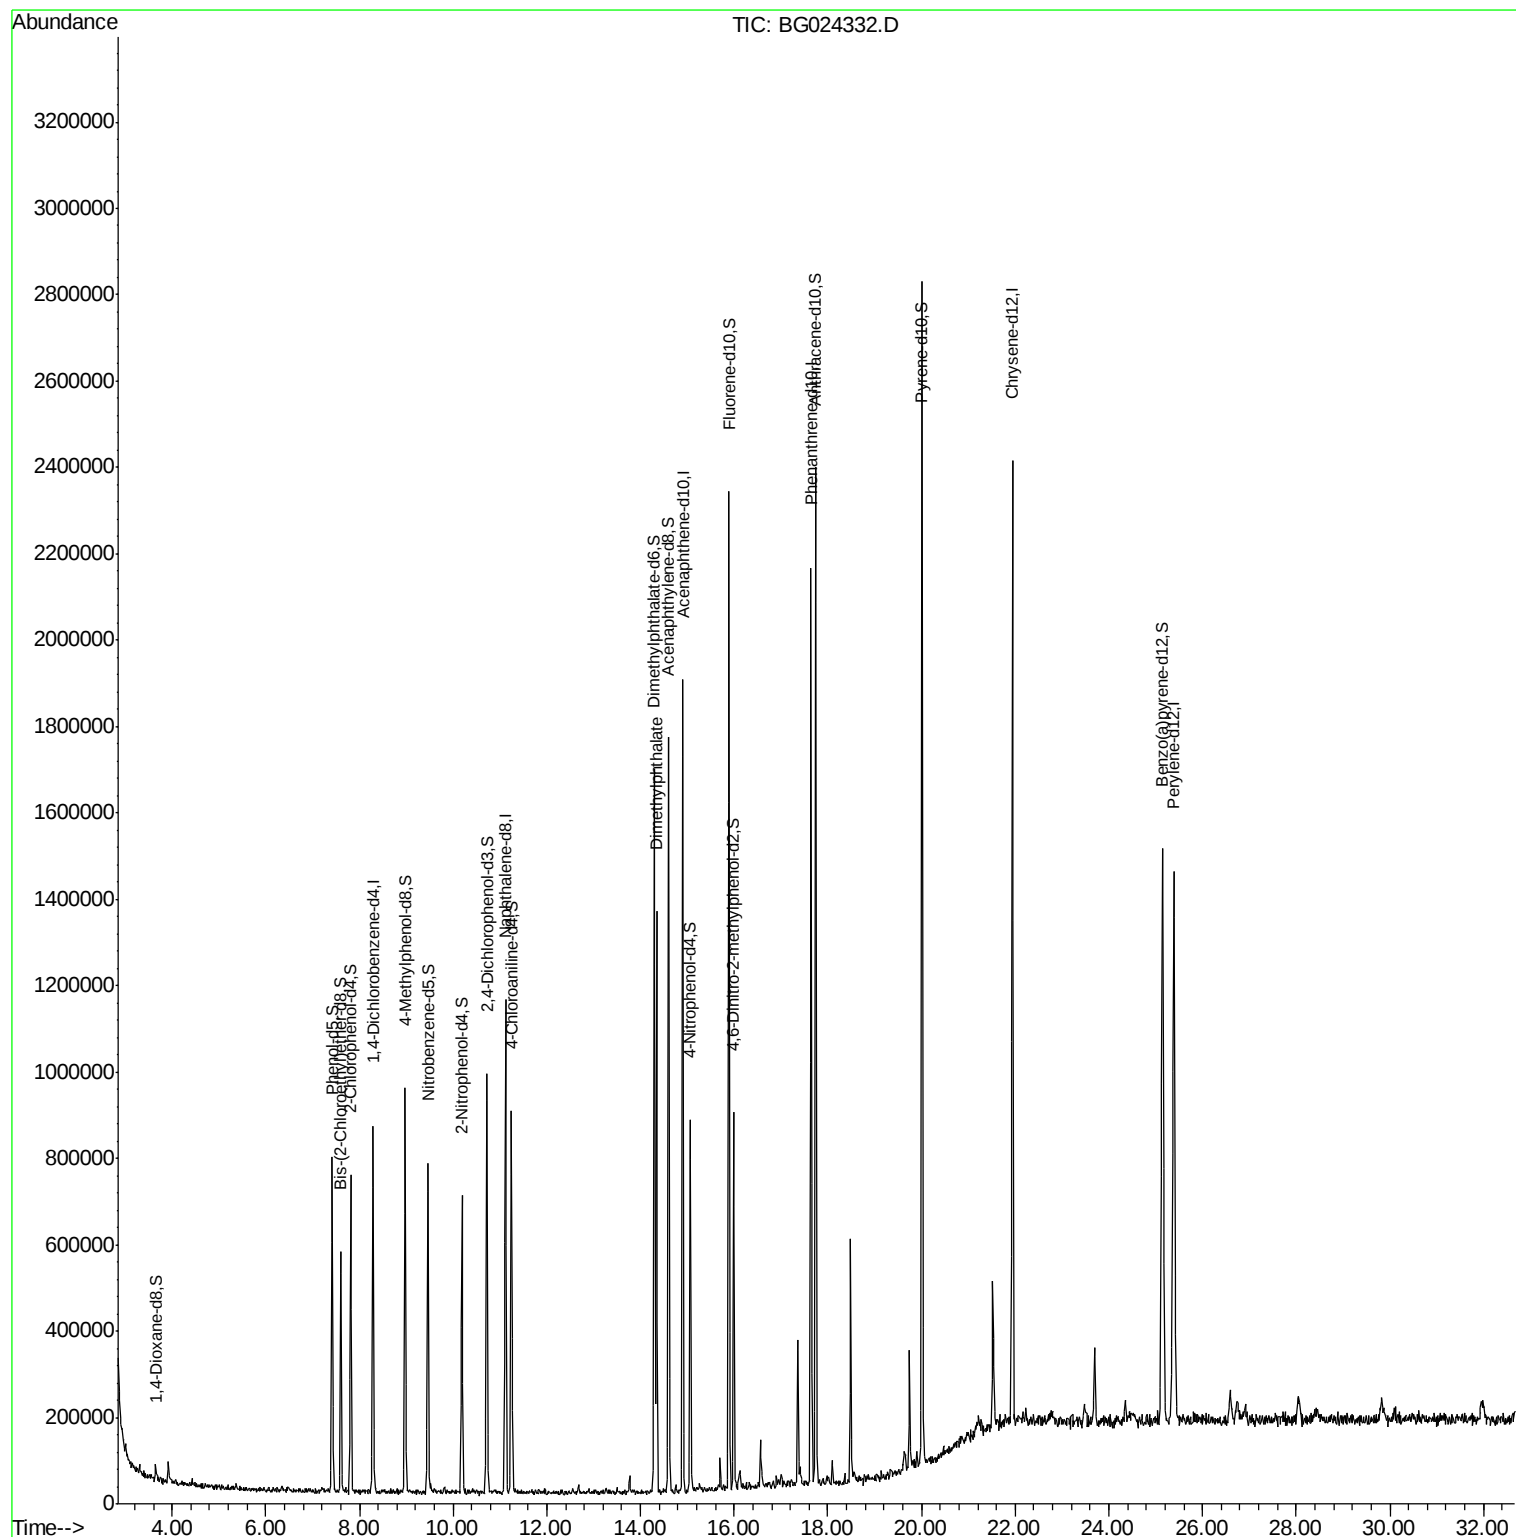

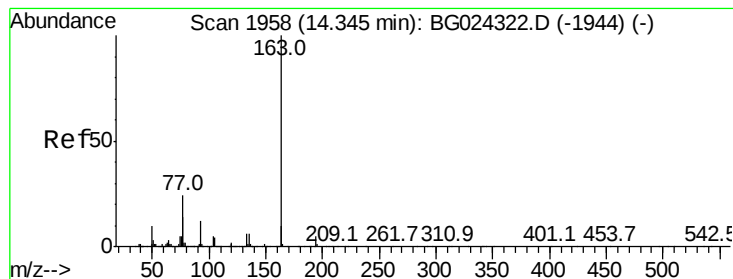

#44

Dimethylphthalate

Concen: 16.73 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. 0.00 min

Lab File: BG024332.D

Acq: 13 Oct 2016 22:25

Instrument :

BNA_G

ClientSampleId :

BDNH9


Tot Ion:163 Resp: 791187

Ion Ratio Lower Upper

163 100

194 4.8 3.4 5.0

164 9.2 9.0 13.4

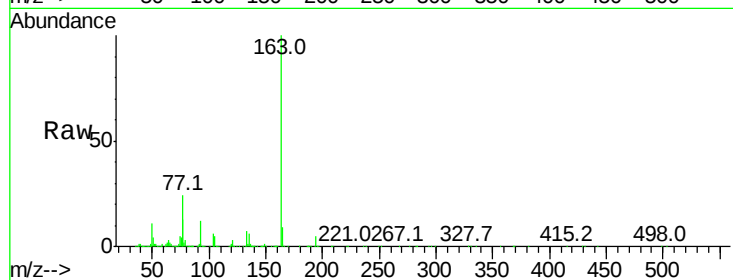

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

