

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024335.D
 Acq On : 14 Oct 2016 00:20
 Operator : UM/SJ
 Sample : H5166-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNJ3

Quant Time: Oct 14 02:33:39 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	228257	20.00	ng/ul	0.00
18) Naphthalene-d8	11.11	136	972417	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	735269	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1384622	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1571125	20.00	ng/ul	0.00
83) Perylene-d12	25.38	264	1631675	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	19536	4.06	ng/uL	0.00
5) Phenol-d5	7.41	99	534872	25.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	345143	23.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	377064	25.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	444334	25.81	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	201539	29.20	ng/ul	0.00
22) 2-Nitrophenol-d4	10.18	143	226645	29.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	434220	25.82	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	535504	30.31	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1346694	26.23	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1595445	27.13	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	227408	24.98	ng/ul	0.00
57) Fluorene-d10	15.89	176	1233702	25.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	244078	29.33	ng/ul	0.00
70) Anthracene-d10	17.74	188	1718377	27.47	ng/ul	0.00
76) Pyrene-d10	20.01	212	1963130	26.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	2087717	28.44	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.34	163	927728	18.43	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024335.D
Acq On : 14 Oct 2016 00:20
Operator : UM/SJ
Sample : H5166-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNJ3

Quant Time: Oct 14 02:33:39 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

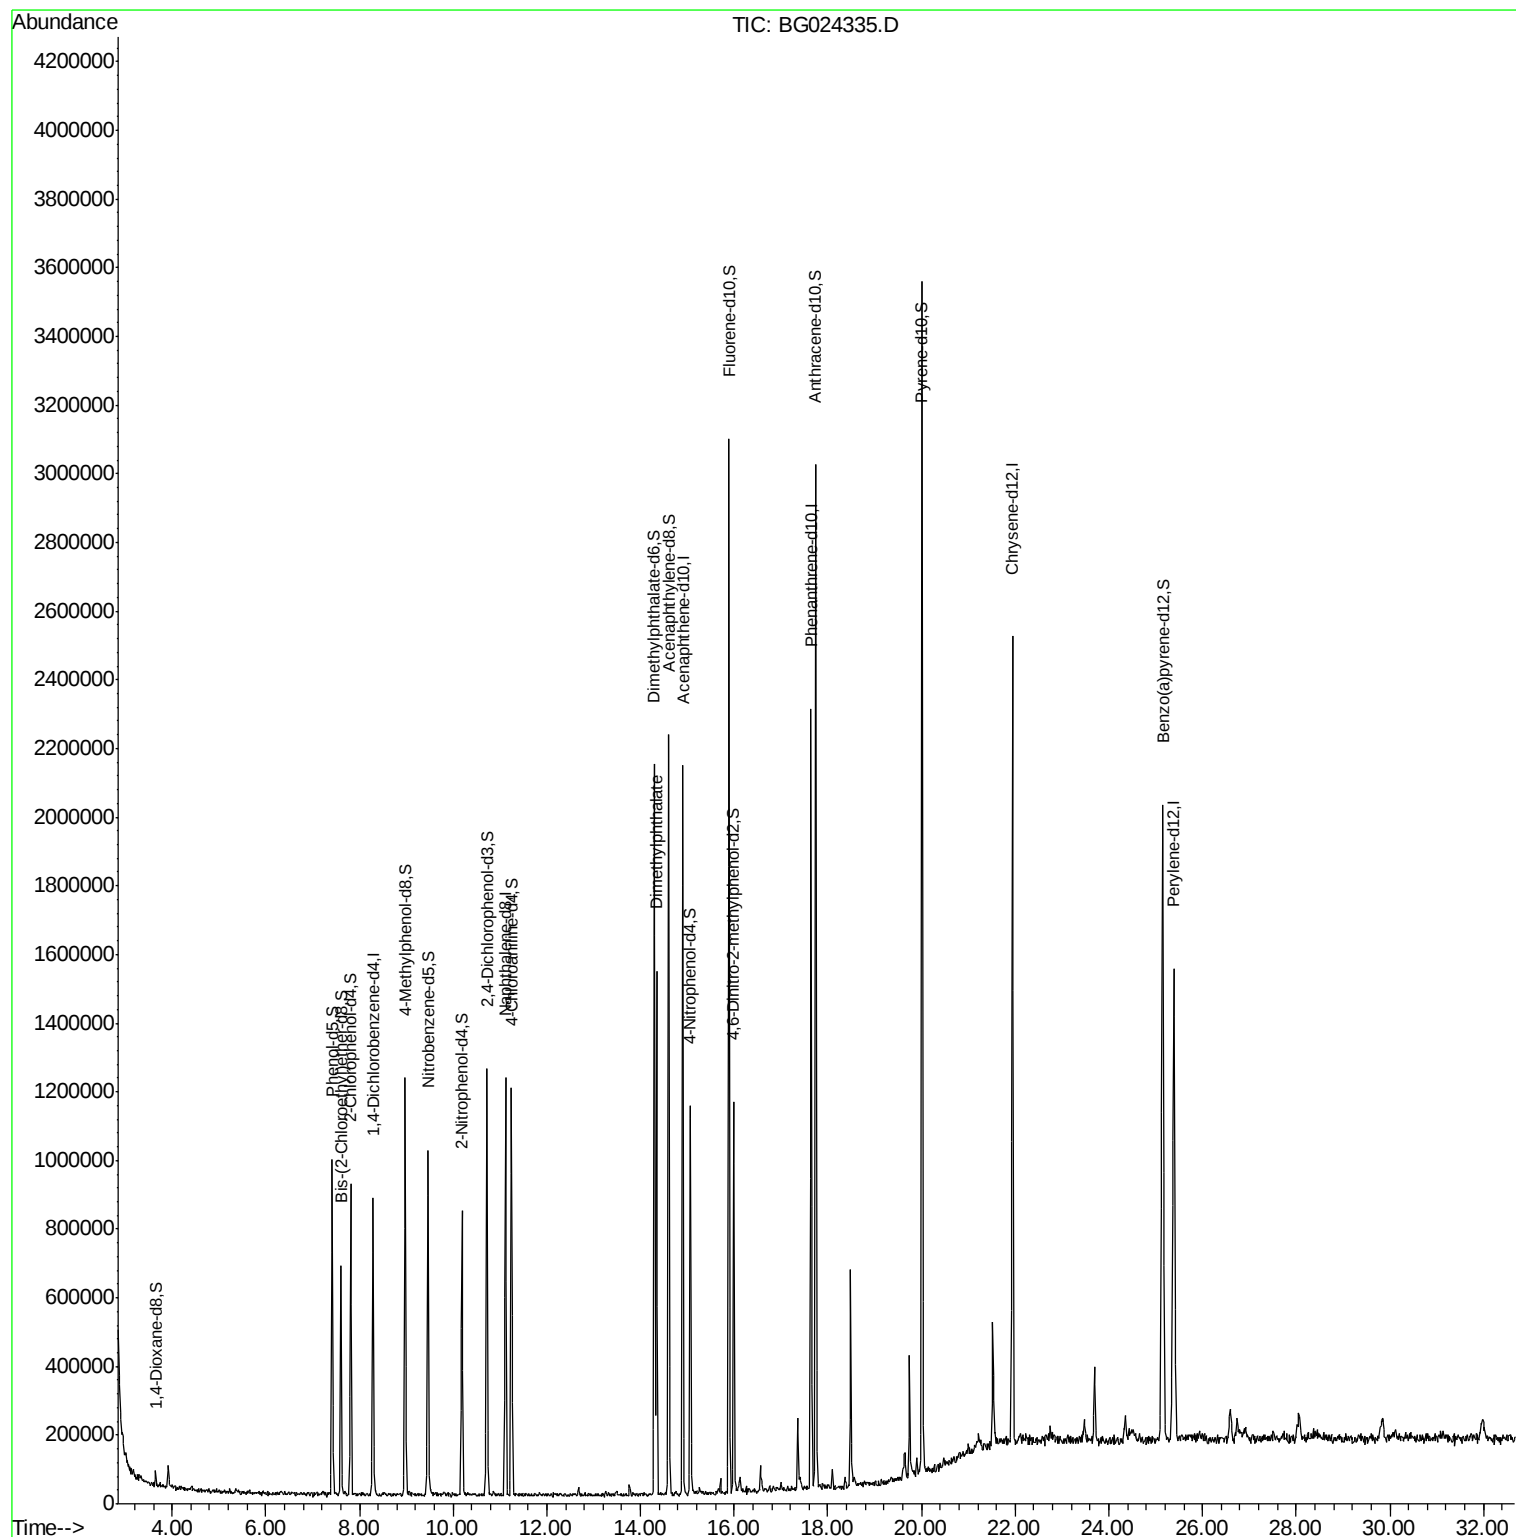

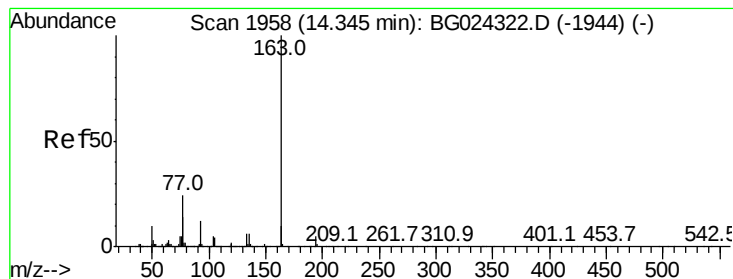

#44

Dimethylphthalate

Concen: 18.43 ng/ul

RT: 14.34 min Scan# 1958

Delta R.T. 0.00 min

Lab File: BG024335.D

Acq: 14 Oct 2016 00:20

Instrument :

BNA_G

ClientSampleId :

BDNJ3

Tot Ion:163 Resp: 927728

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.6 9.0 13.4

