

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
 Data File : BG024336.D
 Acq On : 14 Oct 2016 00:58
 Operator : UM/SJ
 Sample : H5166-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNJ5

Quant Time: Oct 14 02:33:49 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 14 02:32:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	249218	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	1079622	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.90	164	824403	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.64	188	1539241	20.00	ng/ul	0.00
75) Chrysene-d12	21.94	240	1749195	20.00	ng/ul	0.00
83) Perylene-d12	25.39	264	1821237	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	21648	4.13	ng/uL	0.00
5) Phenol-d5	7.42	99	554426	23.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.60	67	358938	22.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	383944	23.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	462093	24.58	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	210558	27.48	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	240734	28.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.72	165	464040	24.86	ng/ul	0.00
29) 4-Chloroaniline-d4	11.24	131	565983	28.85	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	1428831	24.82	ng/ul	0.00
46) Acenaphthylene-d8	14.60	160	1682013	25.51	ng/ul	0.00
51) 4-Nitrophenol-d4	15.06	143	241631	23.67	ng/ul	0.00
57) Fluorene-d10	15.89	176	1331728	24.47	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	259309	28.03	ng/ul	0.00
70) Anthracene-d10	17.74	188	1829553	26.31	ng/ul	0.00
76) Pyrene-d10	20.01	212	2049591	25.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.15	264	2210893	26.98	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.34	163	827983	14.67	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101316\
Data File : BG024336.D
Acq On : 14 Oct 2016 00:58
Operator : UM/SJ
Sample : H5166-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNJ5

Quant Time: Oct 14 02:33:49 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 14 02:32:10 2016
Response via : Initial Calibration

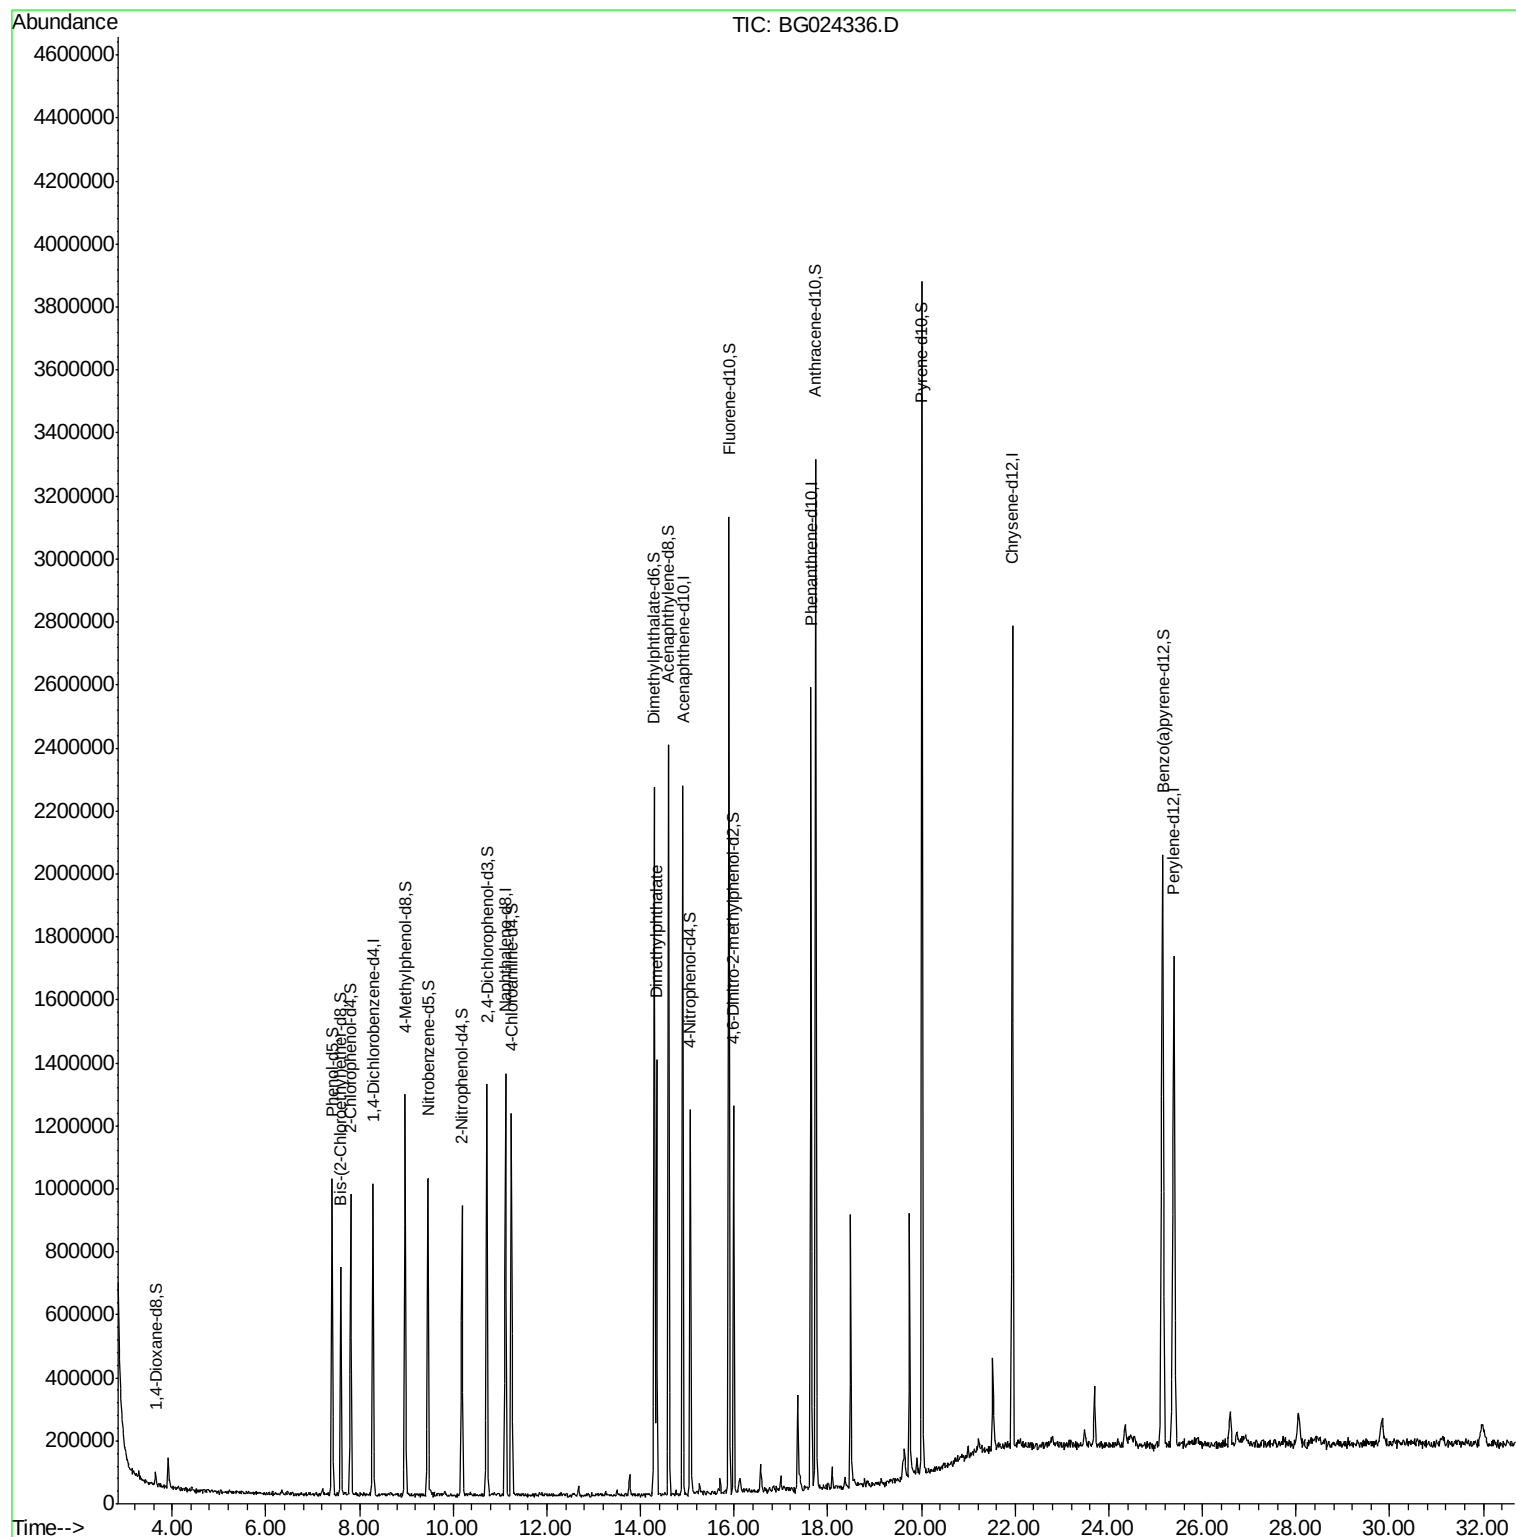

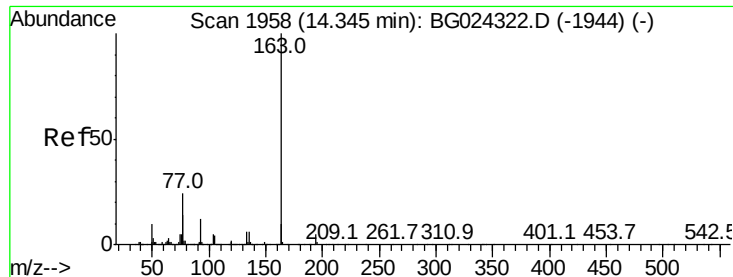

#44

Dimethylphthalate

Concen: 14.67 ng/ul

RT: 14.34 min Scan# 1957

Delta R.T. -0.00 min

Lab File: BG024336.D

Acq: 14 Oct 2016 00:58

Instrument :

BNA_G

ClientSampleId :

BDNJ5


Tot Ion:163 Resp: 827983

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 11.3 9.0 13.4

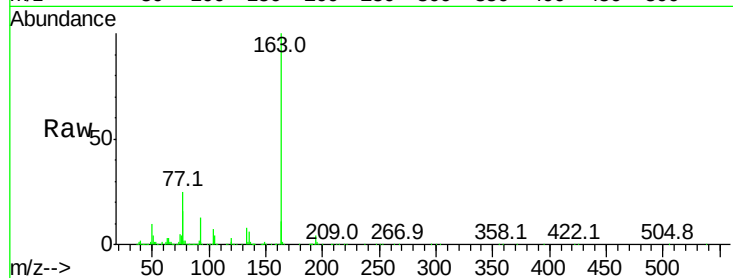

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

