
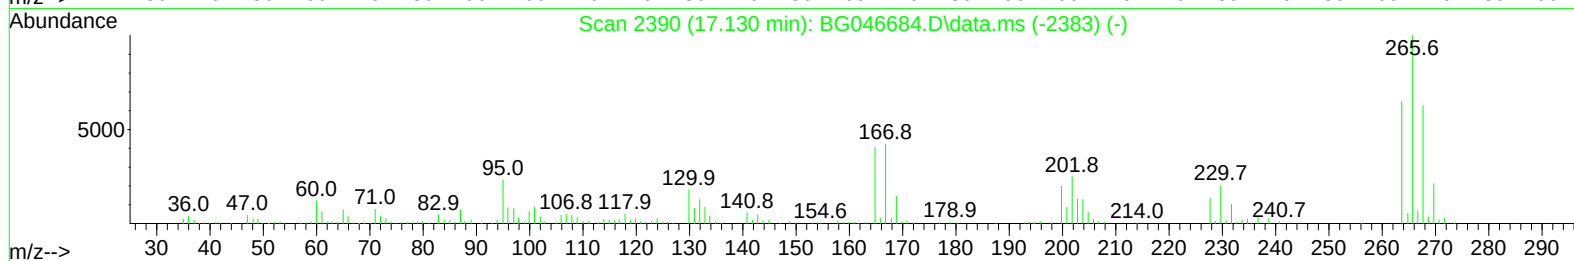
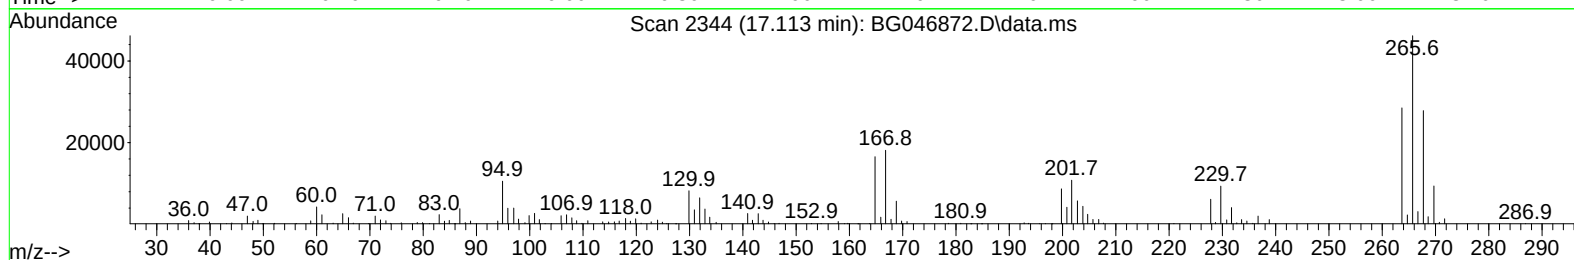


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101320\
Data File : BG046872.D
Acq On : 13 Oct 2020 13:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 03:12:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

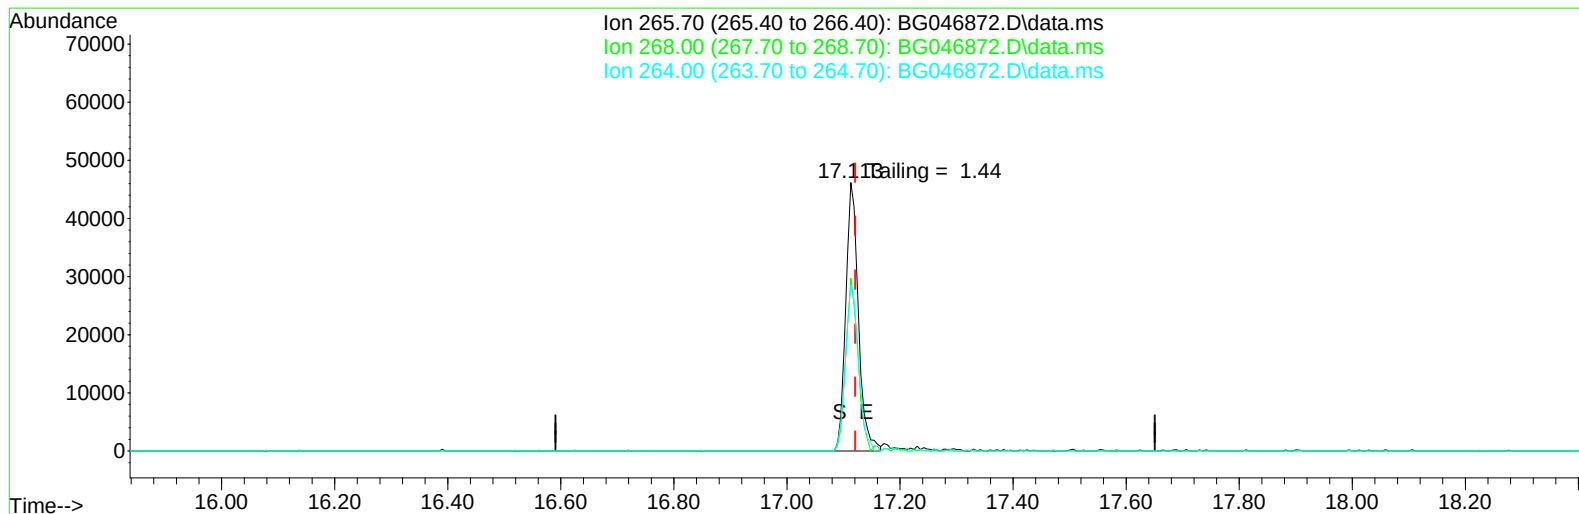

TIC: BG046872.D\data.ms

(70) Pentachlorophenol (C)




17.113min (-0.008) 20603.63 ng

response 71953

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.36
264.00	61.60	66.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101320\
Data File : BG046872.D
Acq On : 13 Oct 2020 13:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 03:12:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

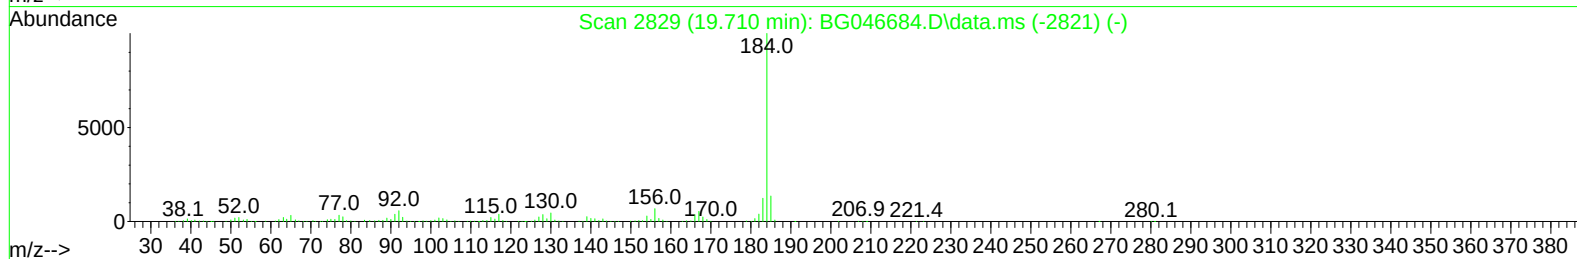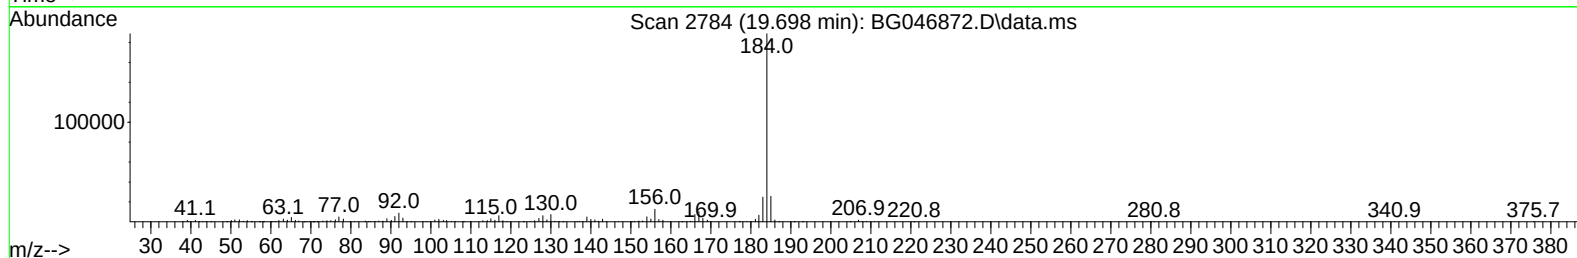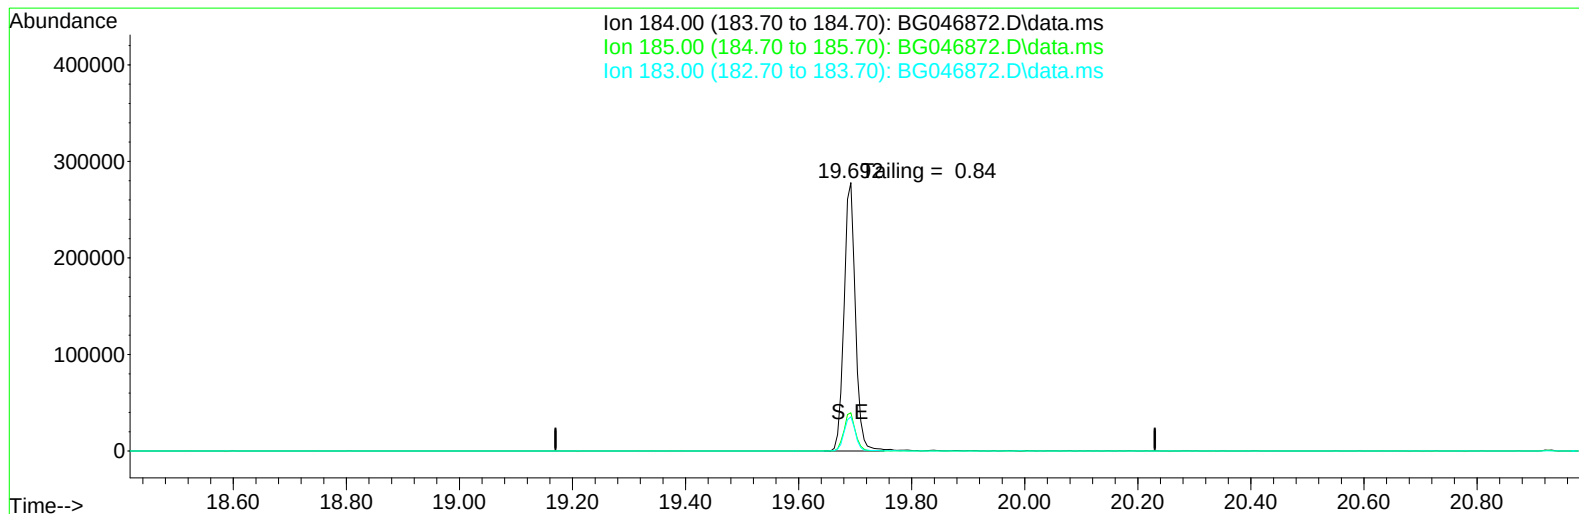

TIC: BG046872.D\data.ms

(77) Benzidine

19.700min (-19.700) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.50	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00