
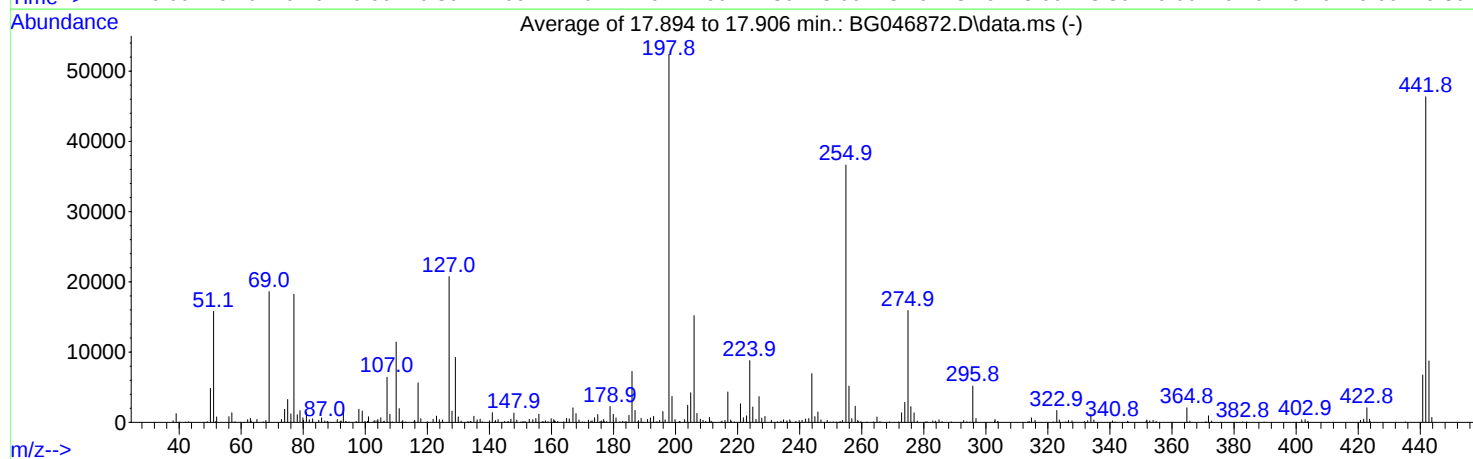


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101320\
 Data File : BG046872.D
 Acq On : 13 Oct 2020 13:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 11:38:17 2020

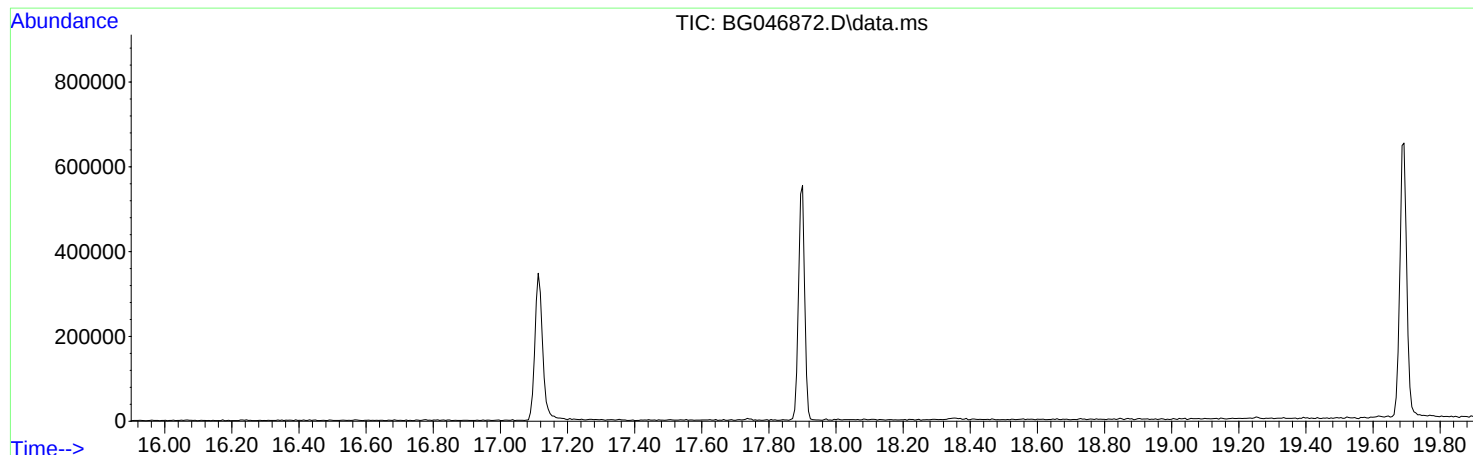

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	15800	PASS
68	69	0.00	2	1.5	272	PASS
69	198	0.00	100	35.5	18608	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.6	20743	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52360	PASS
199	198	5	9	7.1	3696	PASS
275	198	10	60	30.4	15917	PASS
365	198	1	100	4.0	2074	PASS
441	198	0.01	100	12.9	6747	PASS
442	198	50	100	88.5	46349	PASS
443	442	15	24	18.9	8742	PASS