
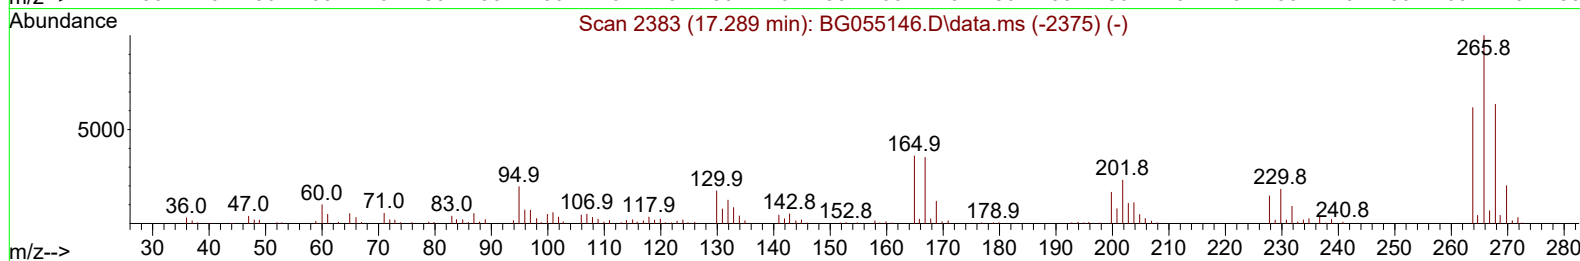
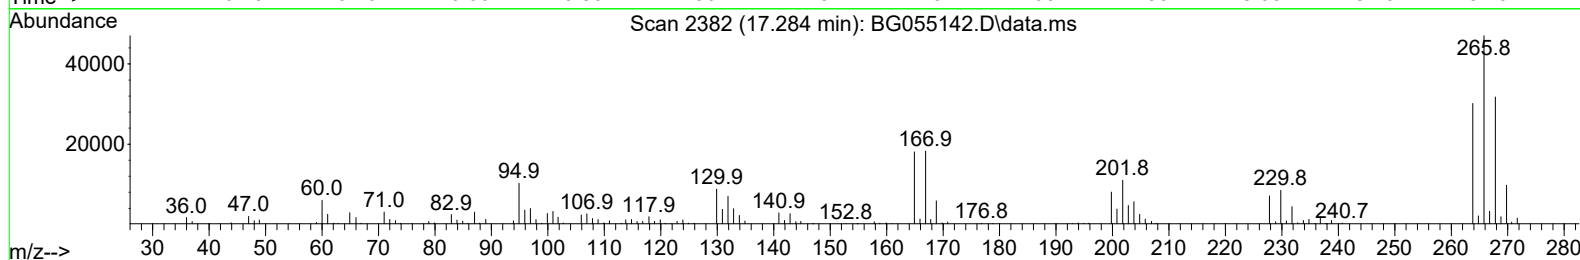


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055142.D
Acq On : 12 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 06:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

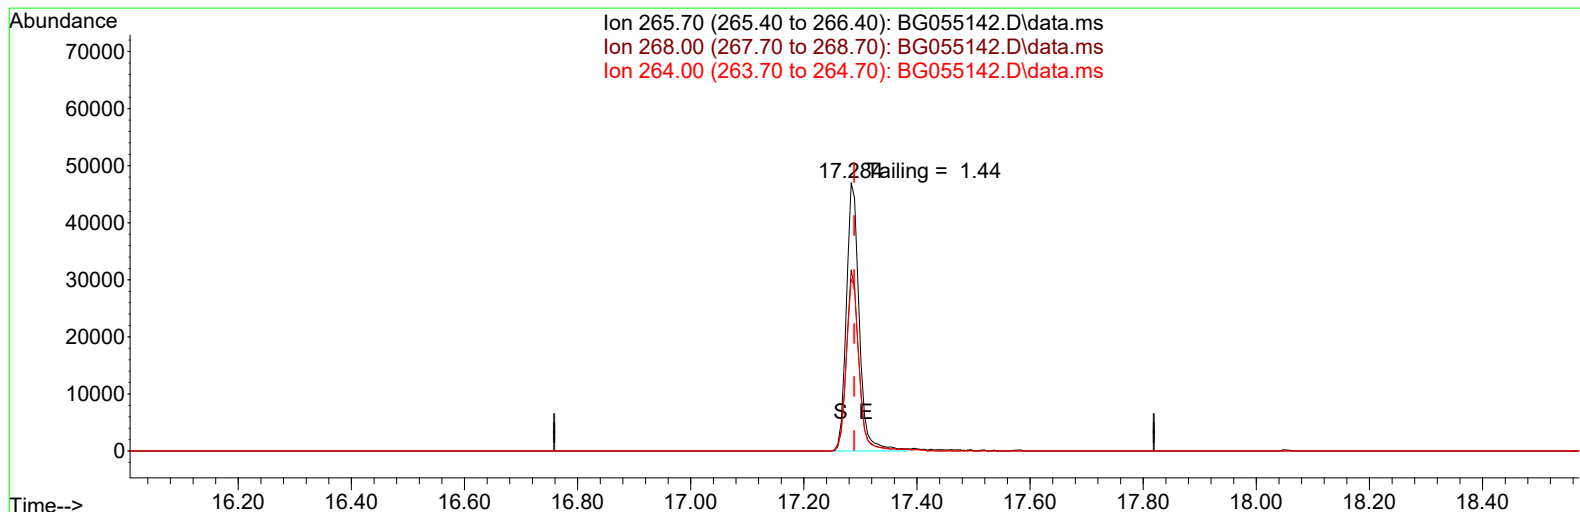

TIC: BG055142.D\data.ms

(70) Pentachlorophenol (C)




17.284min (-0.005) 21927.80 ng

response 74481

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	67.48
264.00	65.90	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055142.D
Acq On : 12 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 06:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

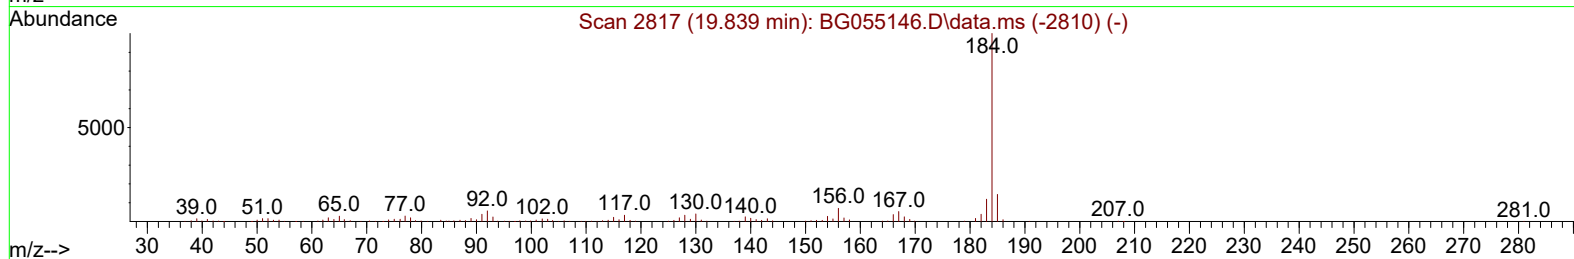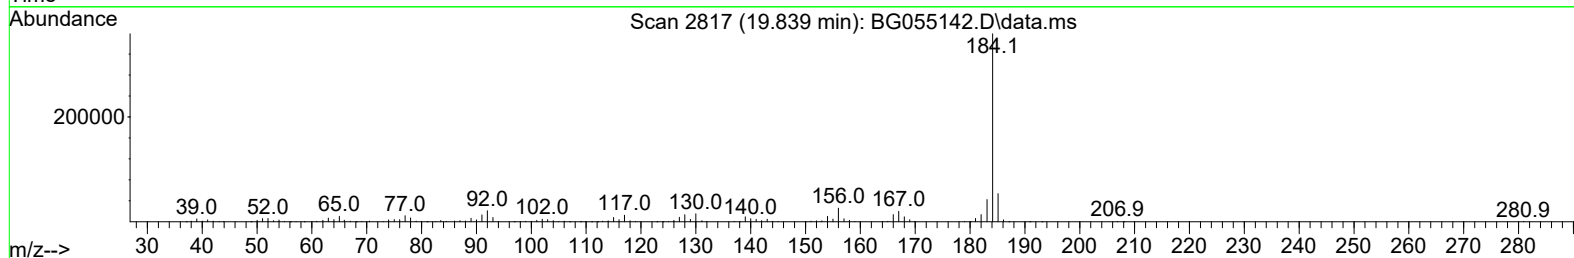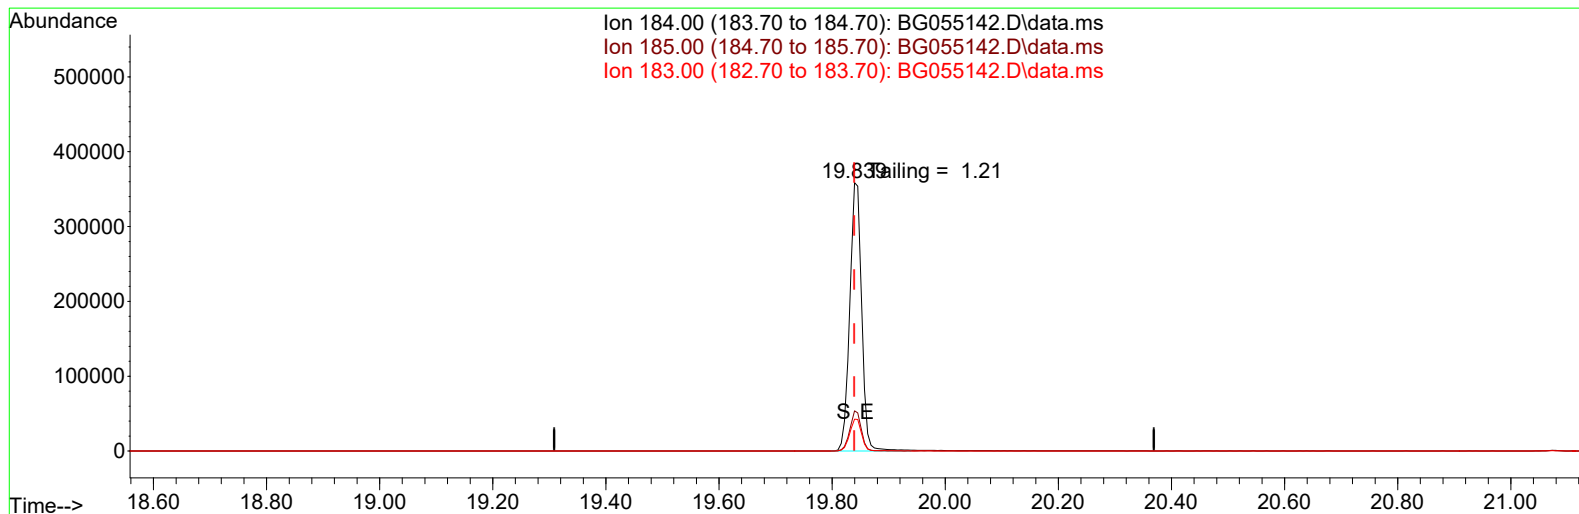

TIC: BG055142.D\data.ms

(77) Benzidine**19.839min (+ 0.001) 28871.85 ng****response 526382**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.99
183.00	11.80	11.89
0.00	0.00	0.00