
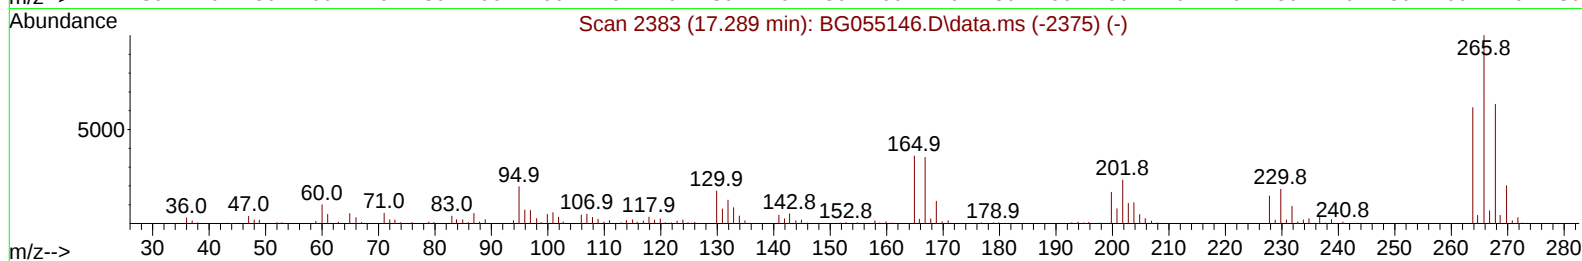
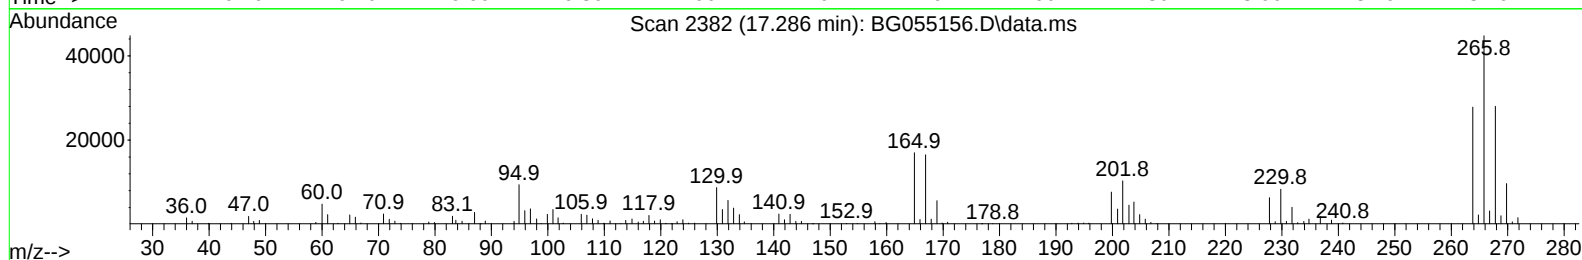


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055156.D
Acq On : 13 Oct 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 02:38:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

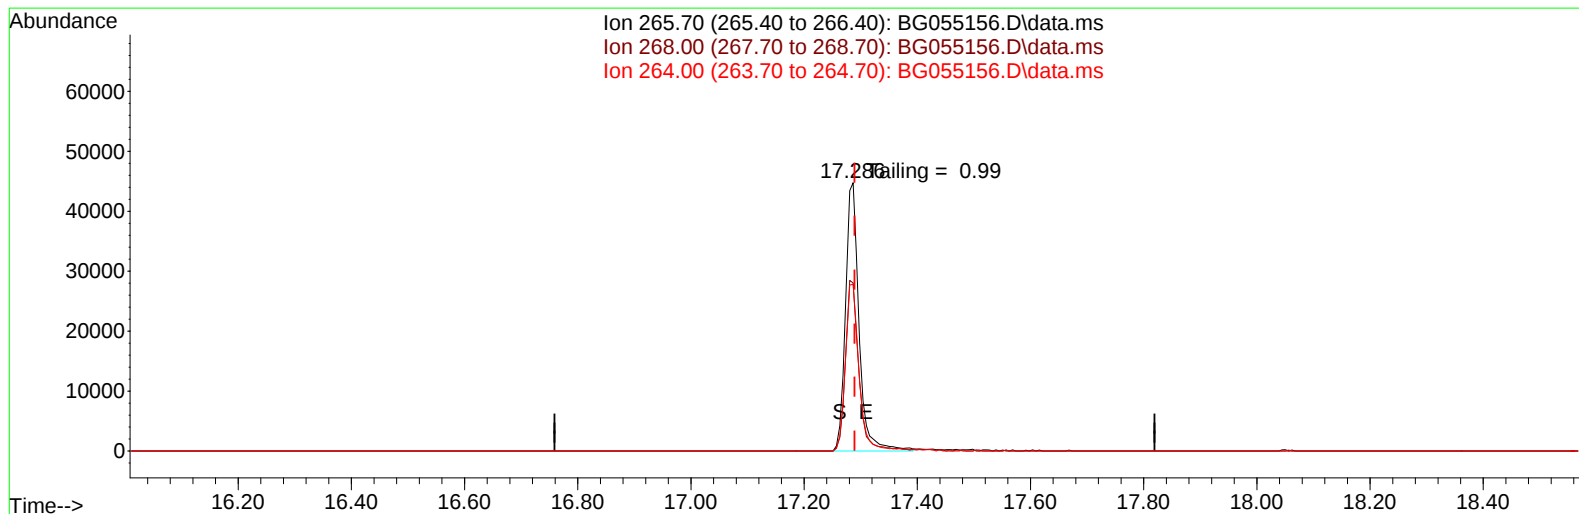

TIC: BG055156.D\data.ms

(70) Pentachlorophenol (C)




17.286min (-0.002) 31451.51 ng

response 73959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	62.60
264.00	65.90	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055156.D
Acq On : 13 Oct 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 14 02:38:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

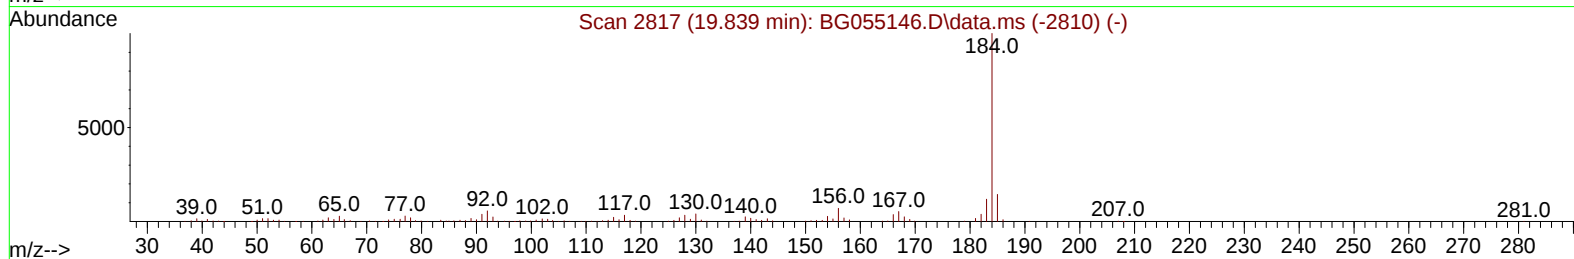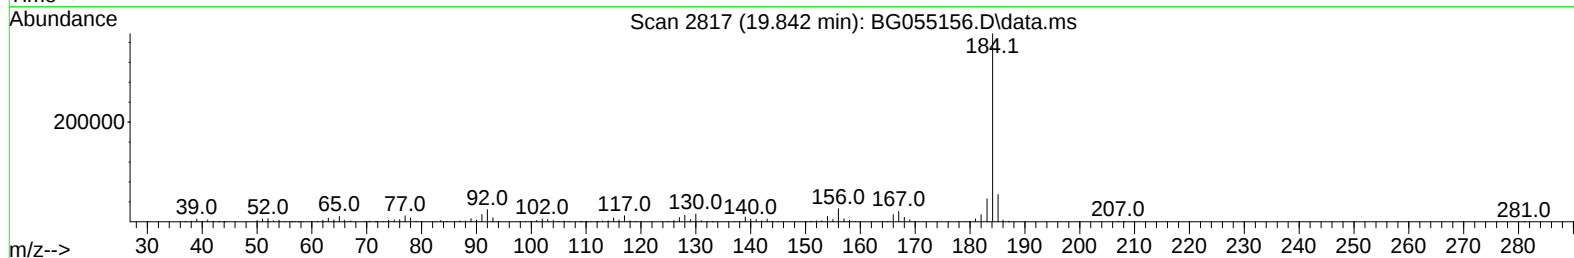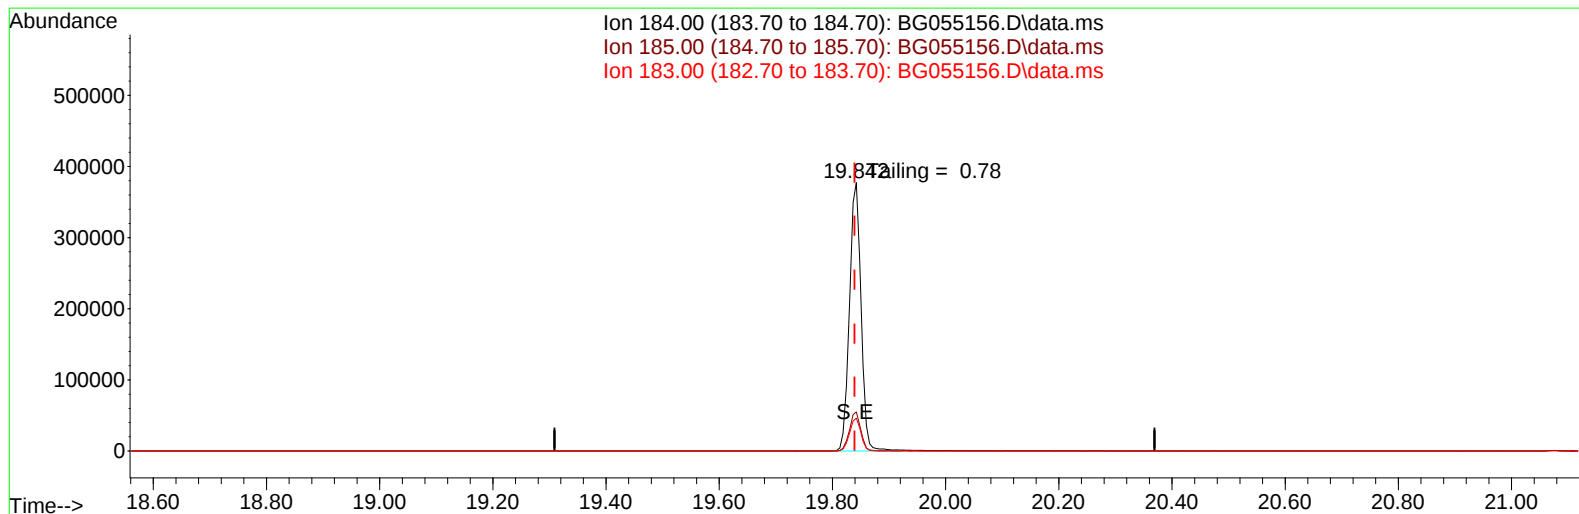

TIC: BG055156.D\data.ms

(77) Benzidine**19.842min (+ 0.003) 53426.54 ng****response 540343**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.54
183.00	11.80	12.21
0.00	0.00	0.00