

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
 Data File : BG055164.D
 Acq On : 13 Oct 2022 15:08
 Operator : CG/JU
 Sample : N5082-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FLORENCE-COMP-2-FLORENCE-VOC-2

Quant Time: Oct 14 01:25:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 13 05:14:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.299	152	33027	20.000	ng	0.00
21) Naphthalene-d8	11.131	136	144923	20.000	ng	0.00
39) Acenaphthene-d10	14.909	164	102127	20.000	ng	0.00
64) Phenanthrene-d10	17.641	188	229914	20.000	ng	0.00
76) Chrysene-d12	21.924	240	217001	20.000	ng	0.00
86) Perylene-d12	25.344	264	229705	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.820	112	248617	147.277	ng	0.00
7) Phenol-d6	7.435	99	337853	135.296	ng	0.00
23) Nitrobenzene-d5	9.474	82	219311	81.150	ng	0.00
42) 2,4,6-Tribromophenol	16.389	330	180740	123.166	ng	0.00
45) 2-Fluorobiphenyl	13.540	172	549401	87.878	ng	0.00
79) Terphenyl-d14	20.220	244	877331	81.426	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055164.D
Acq On : 13 Oct 2022 15:08
Operator : CG/JU
Sample : N5082-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2

Quant Time: Oct 14 01:25:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration




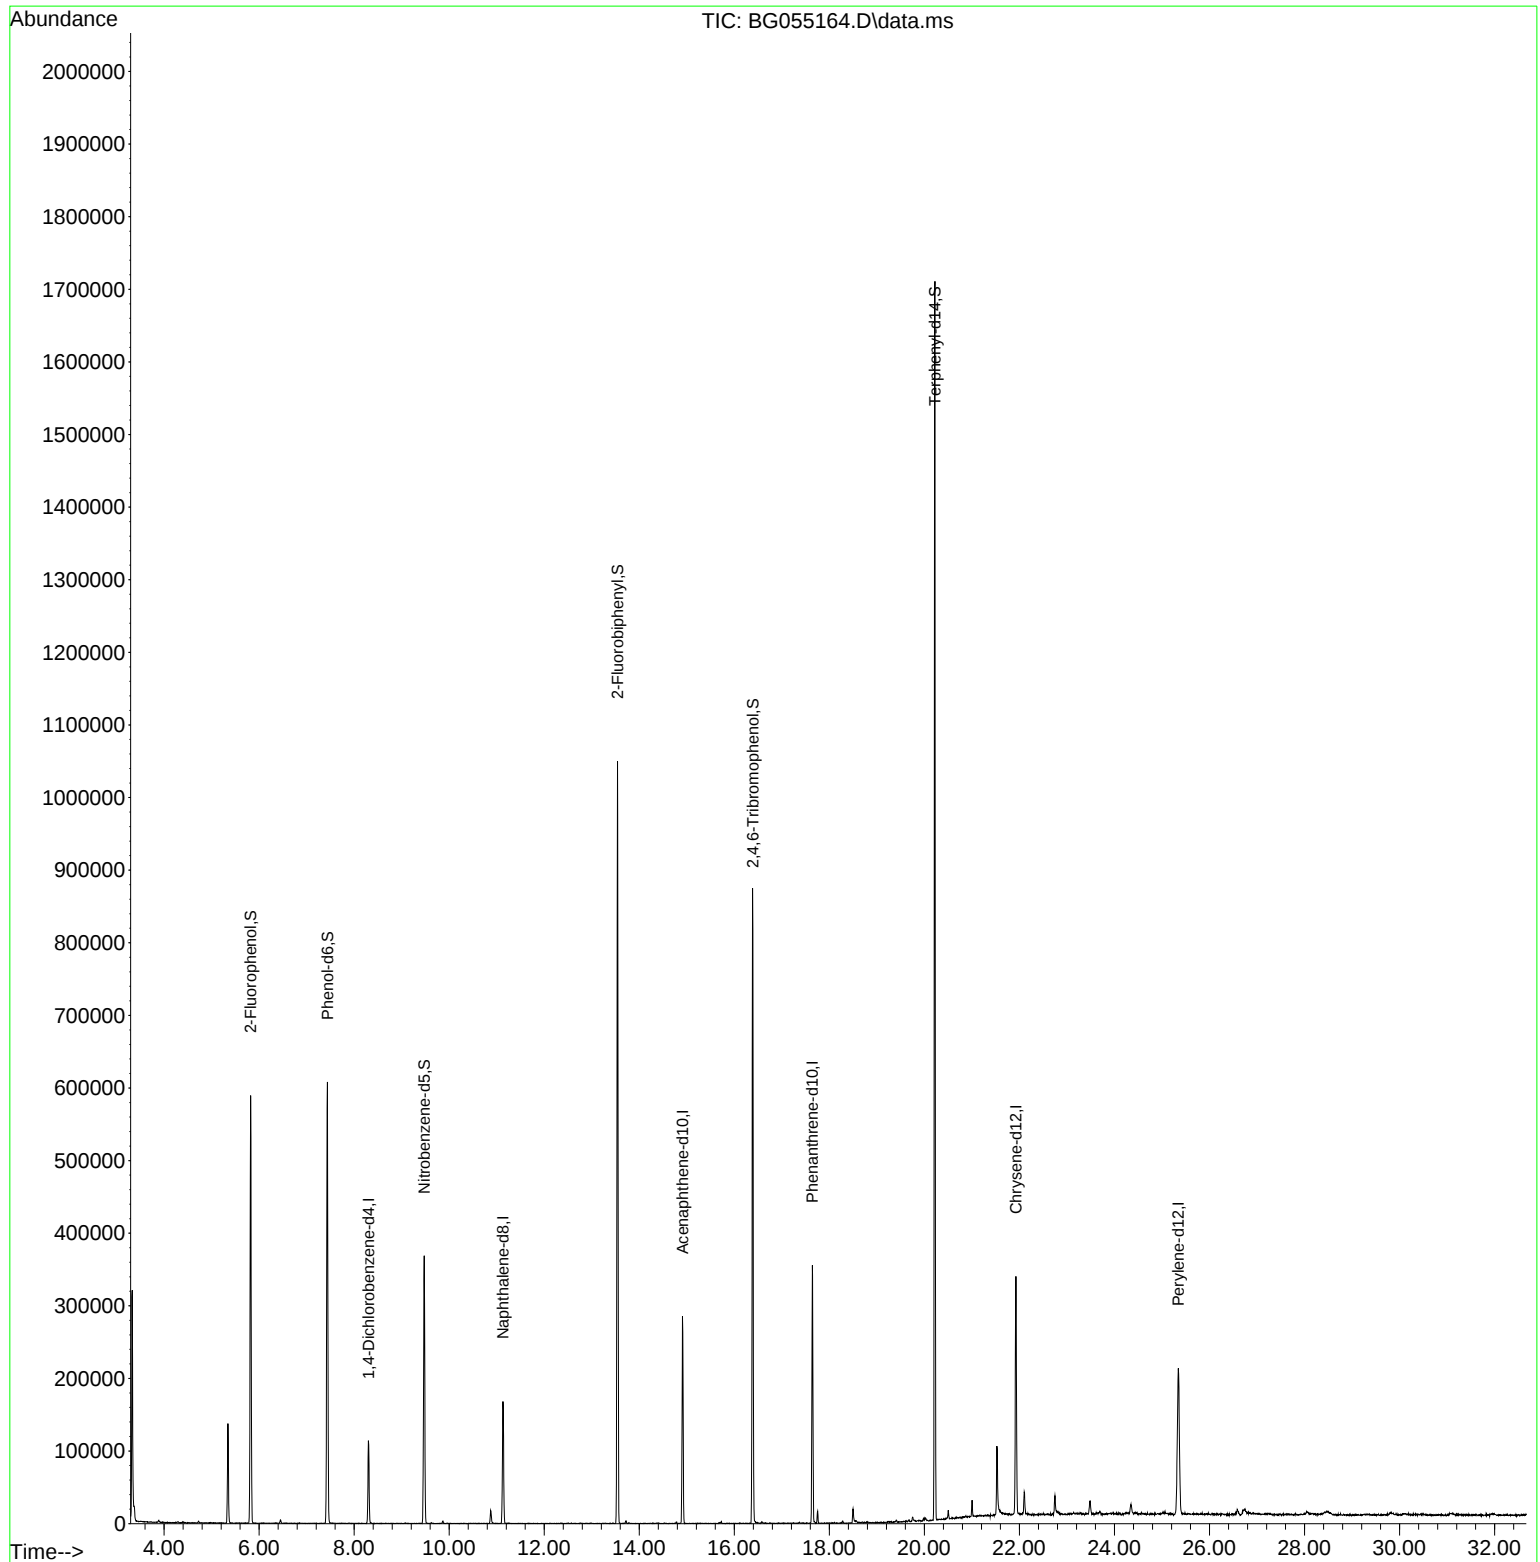


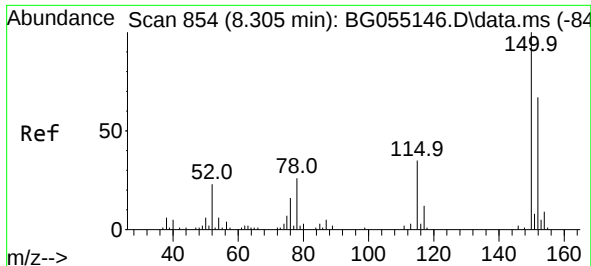

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.299 min Scan# 81
Delta R.T. -0.006 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08




Instrument :
BNA_G
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2


Tgt Ion:152 Resp: 33027
Ion Ratio Lower Upper
152 100
150 158.8 119.7 179.5
115 59.0 42.4 63.6

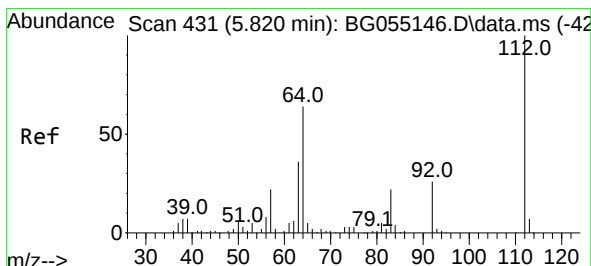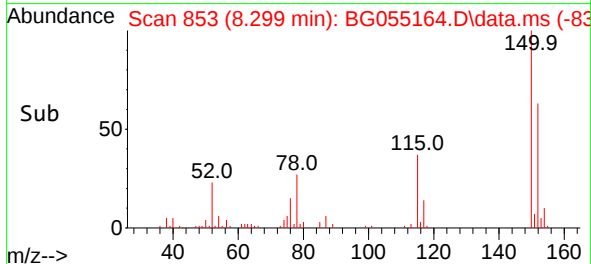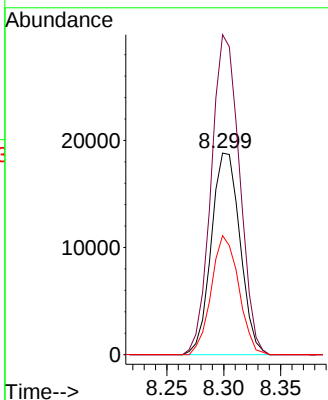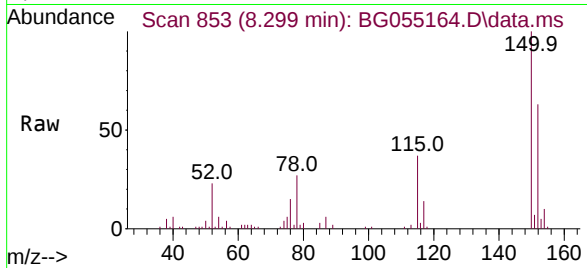

#5
2-Fluorophenol
Concen: 147.277 ng
RT: 5.820 min Scan# 431
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08

Tgt Ion:112 Resp: 248617
Ion Ratio Lower Upper
112 100
64 63.1 50.9 76.3
63 34.4 29.0 43.6


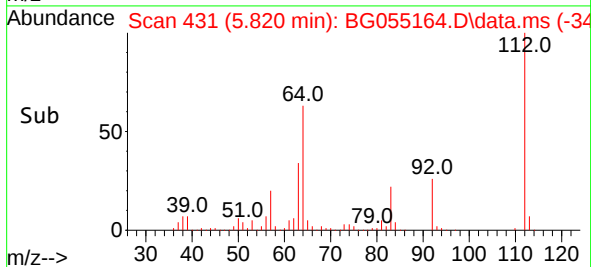
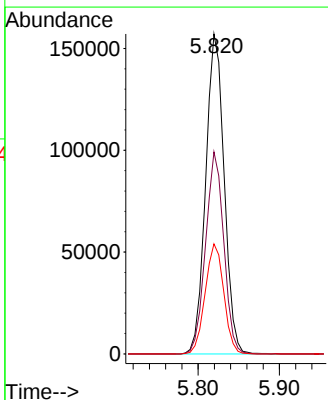
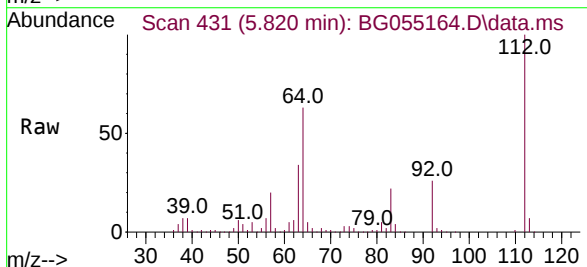


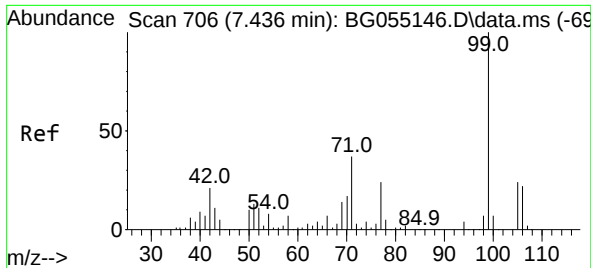

#7
Phenol-d6
Concen: 135.296 ng
RT: 7.435 min Scan# 706
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08




Instrument :
BNA_G
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2


Tgt Ion: 99 Resp: 337853
Ion Ratio Lower Upper
99 100
42 20.4 16.6 25.0
71 37.5 29.6 44.4

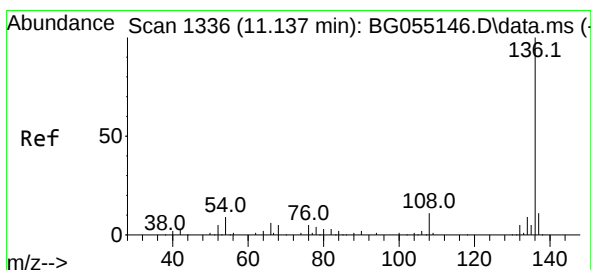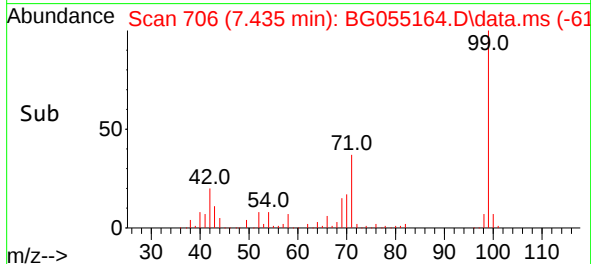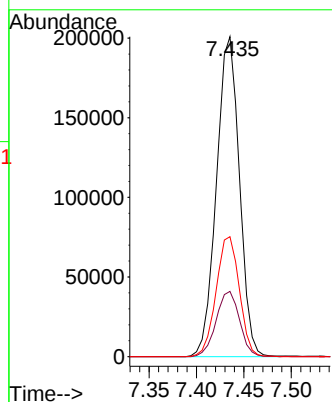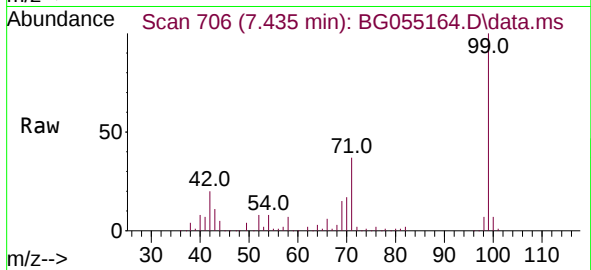

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.131 min Scan# 1335
Delta R.T. -0.006 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08

Tgt Ion:136 Resp: 144923
Ion Ratio Lower Upper
136 100
137 11.8 9.1 13.7
54 9.1 7.0 10.6
68 6.1 4.3 6.5

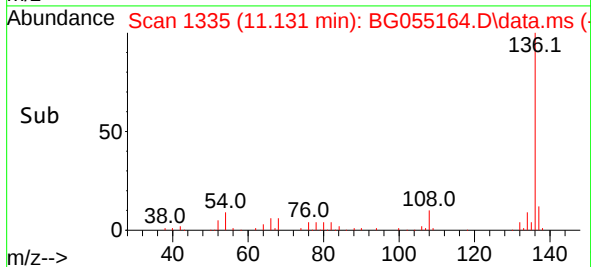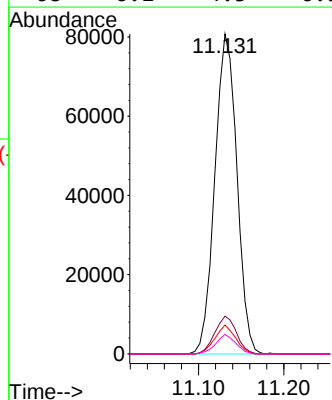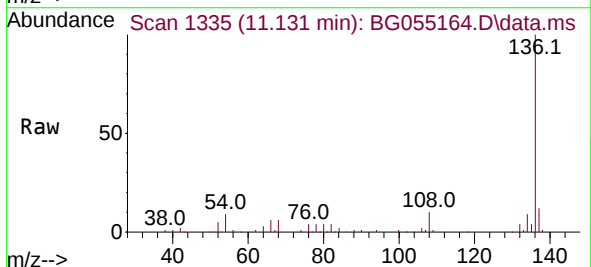

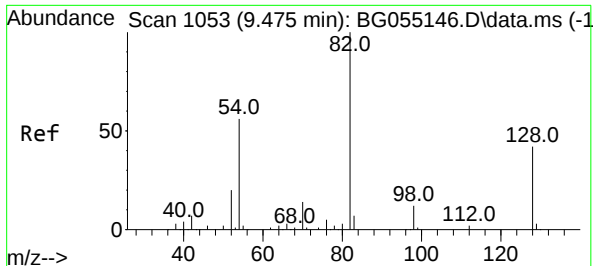

#23

Nitrobenzene-d5

Concen: 81.150 ng

RT: 9.474 min Scan# 1053

Delta R.T. -0.000 min

Lab File: BG055164.D

Acq: 13 Oct 2022 15:08

Instrument :

BNA_G

ClientSampleId :

FLORENCE-COMP-2-FLORENCE-VOC-2





Tgt Ion: 82 Resp: 219311

Ion Ratio Lower Upper

82 100

128 43.1 33.5 50.3

54 54.4 44.7 67.1

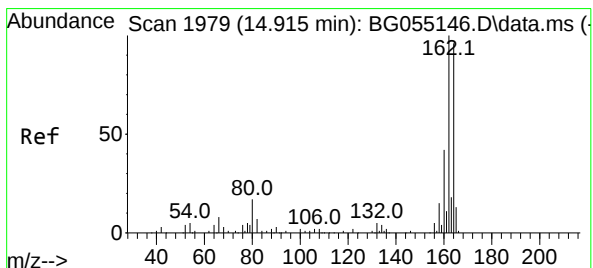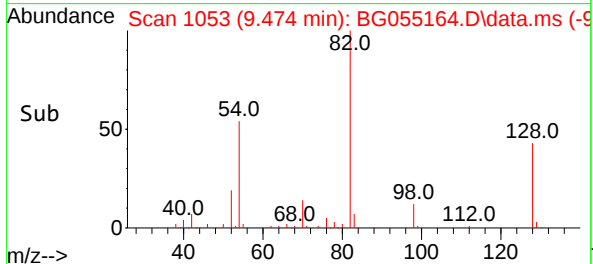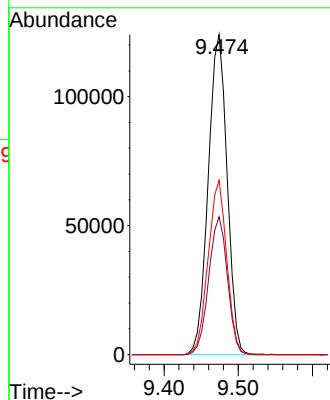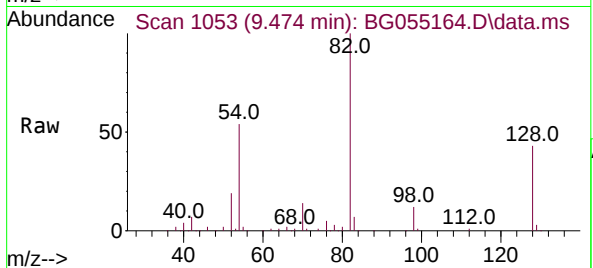

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.909 min Scan# 1978

Delta R.T. -0.006 min

Lab File: BG055164.D

Acq: 13 Oct 2022 15:08




Tgt Ion: 164 Resp: 102127


Ion Ratio Lower Upper

164 100

162 109.2 83.3 124.9

160 46.5 35.3 52.9


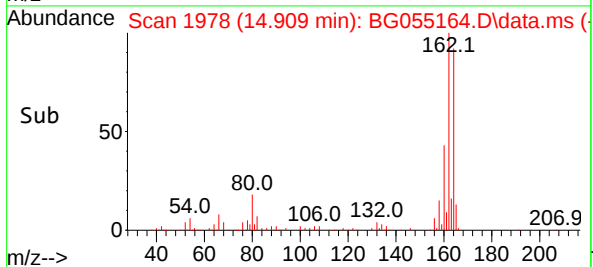
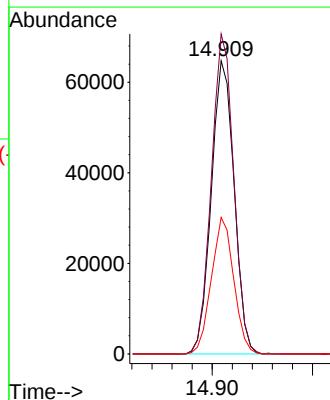
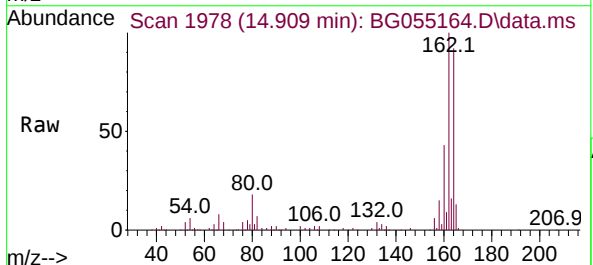


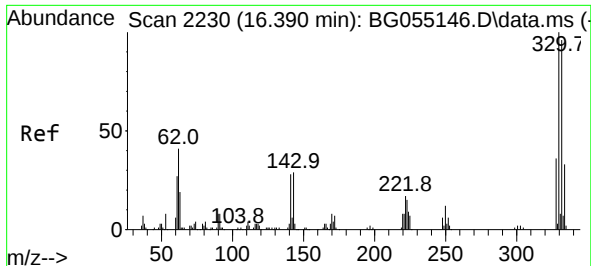

#42
2,4,6-Tribromophenol
Concen: 123.166 ng
RT: 16.389 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08




Instrument :
BNA_G
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2


Tgt Ion:330 Resp: 180740
Ion Ratio Lower Upper
330 100
332 96.2 77.0 115.4
141 30.6 24.6 36.8

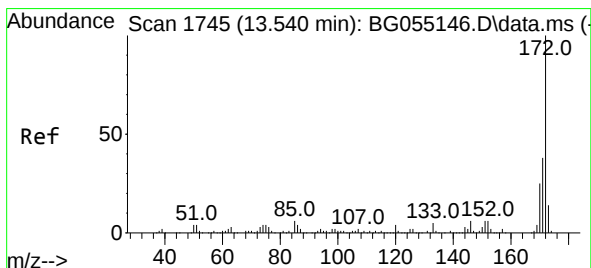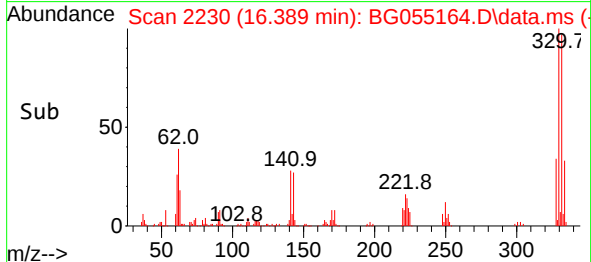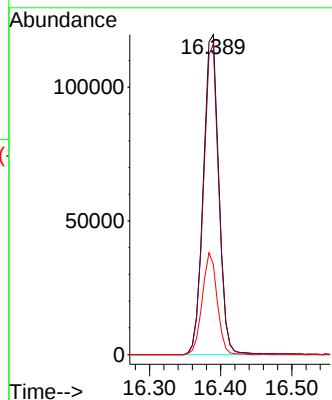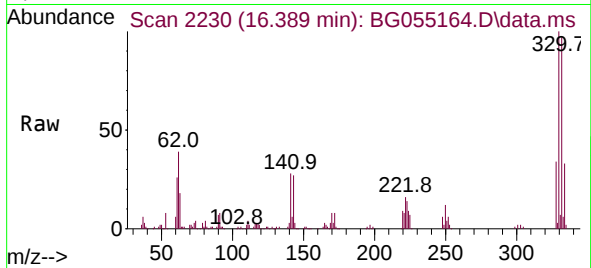

#45
2-Fluorobiphenyl
Concen: 87.878 ng
RT: 13.540 min Scan# 1745
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08

Tgt Ion:172 Resp: 549401
Ion Ratio Lower Upper
172 100
171 36.6 30.1 45.1
170 24.9 19.8 29.6


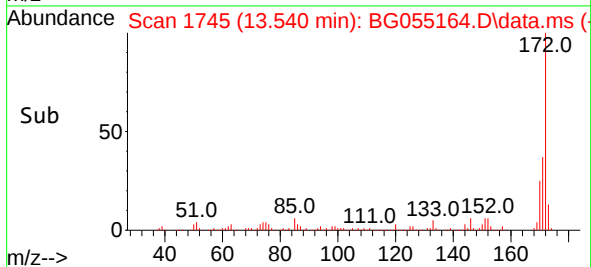
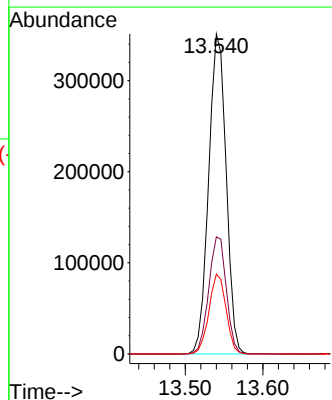
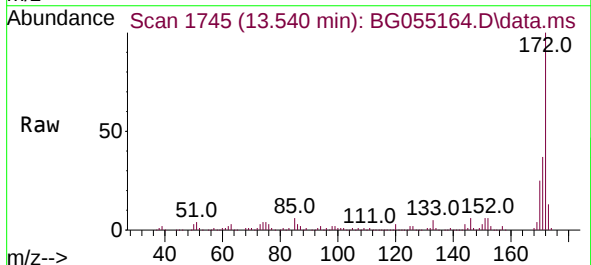


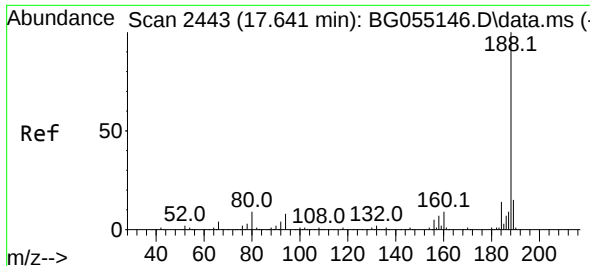

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.641 min Scan# 2443
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08




Instrument :
BNA_G
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2


Tgt Ion:188 Resp: 229914
Ion Ratio Lower Upper
188 100
94 7.5 6.2 9.2
80 8.2 7.0 10.6

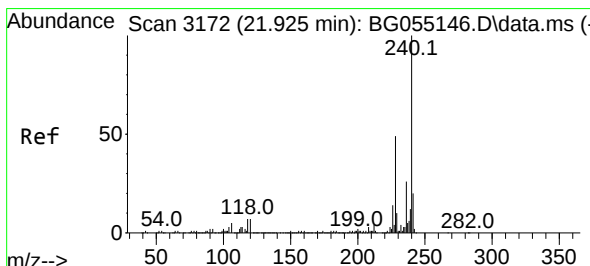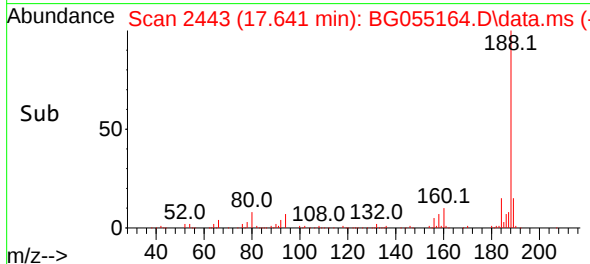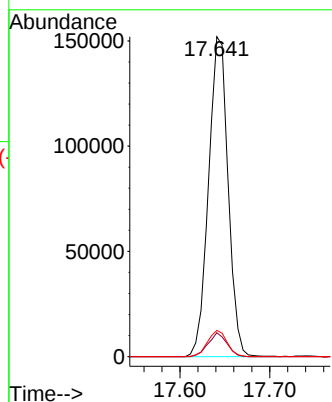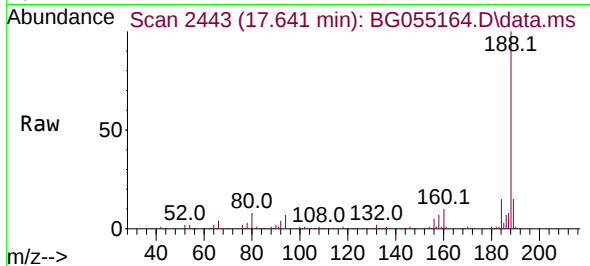

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.924 min Scan# 3172
Delta R.T. -0.000 min
Lab File: BG055164.D
Acq: 13 Oct 2022 15:08

Tgt Ion:240 Resp: 217001
Ion Ratio Lower Upper
240 100
120 7.5 5.4 8.0
236 25.9 20.6 31.0


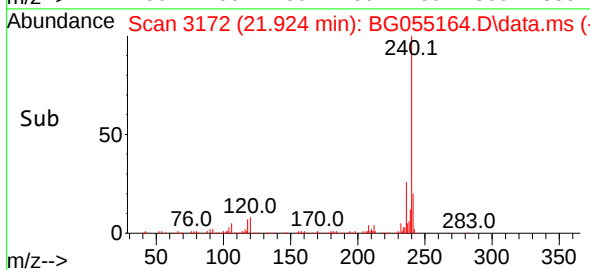
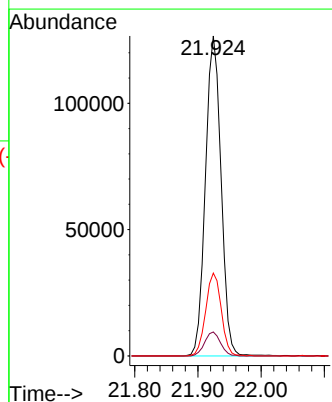
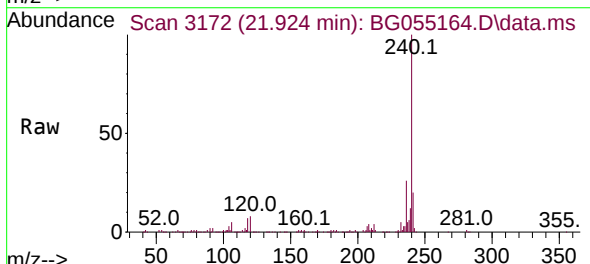


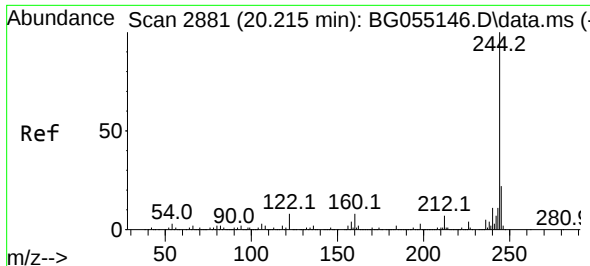

#79
 Terphenyl-d14
 Concen: 81.426 ng
 RT: 20.220 min Scan# 2882
 Delta R.T. 0.005 min
 Lab File: BG055164.D
 Acq: 13 Oct 2022 15:08

Instrument :
 BNA_G
 ClientSampleId :
 FLORENCE-COMP-2-FLORENCE-VOC-2

Tgt Ion:244 Resp: 877331
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.9 8.9
 122 7.5 6.6 10.0

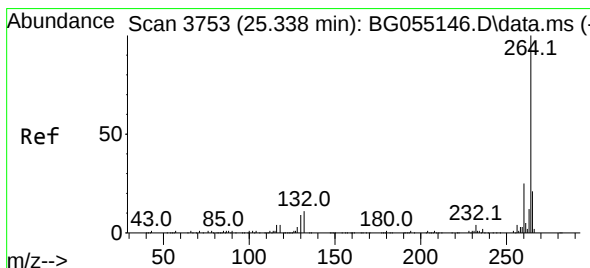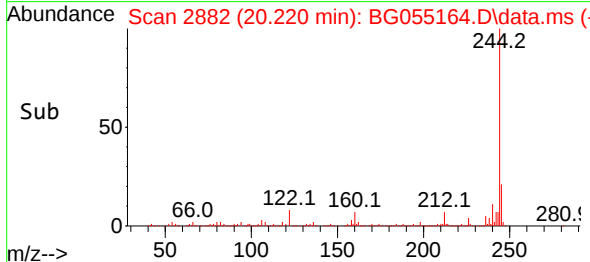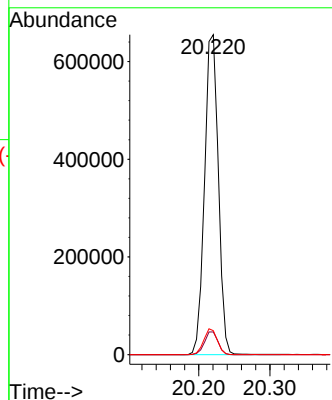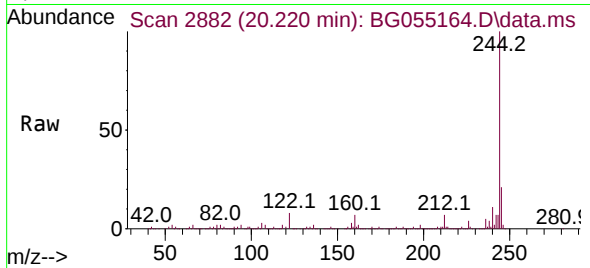

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.344 min Scan# 3754
 Delta R.T. 0.005 min
 Lab File: BG055164.D
 Acq: 13 Oct 2022 15:08

Tgt Ion:264 Resp: 229705
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.1 30.1
 265 21.9 16.8 25.2

