


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
 Data File : BG055142.D
 Acq On : 12 Oct 2022 15:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 13 05:14:13 2022

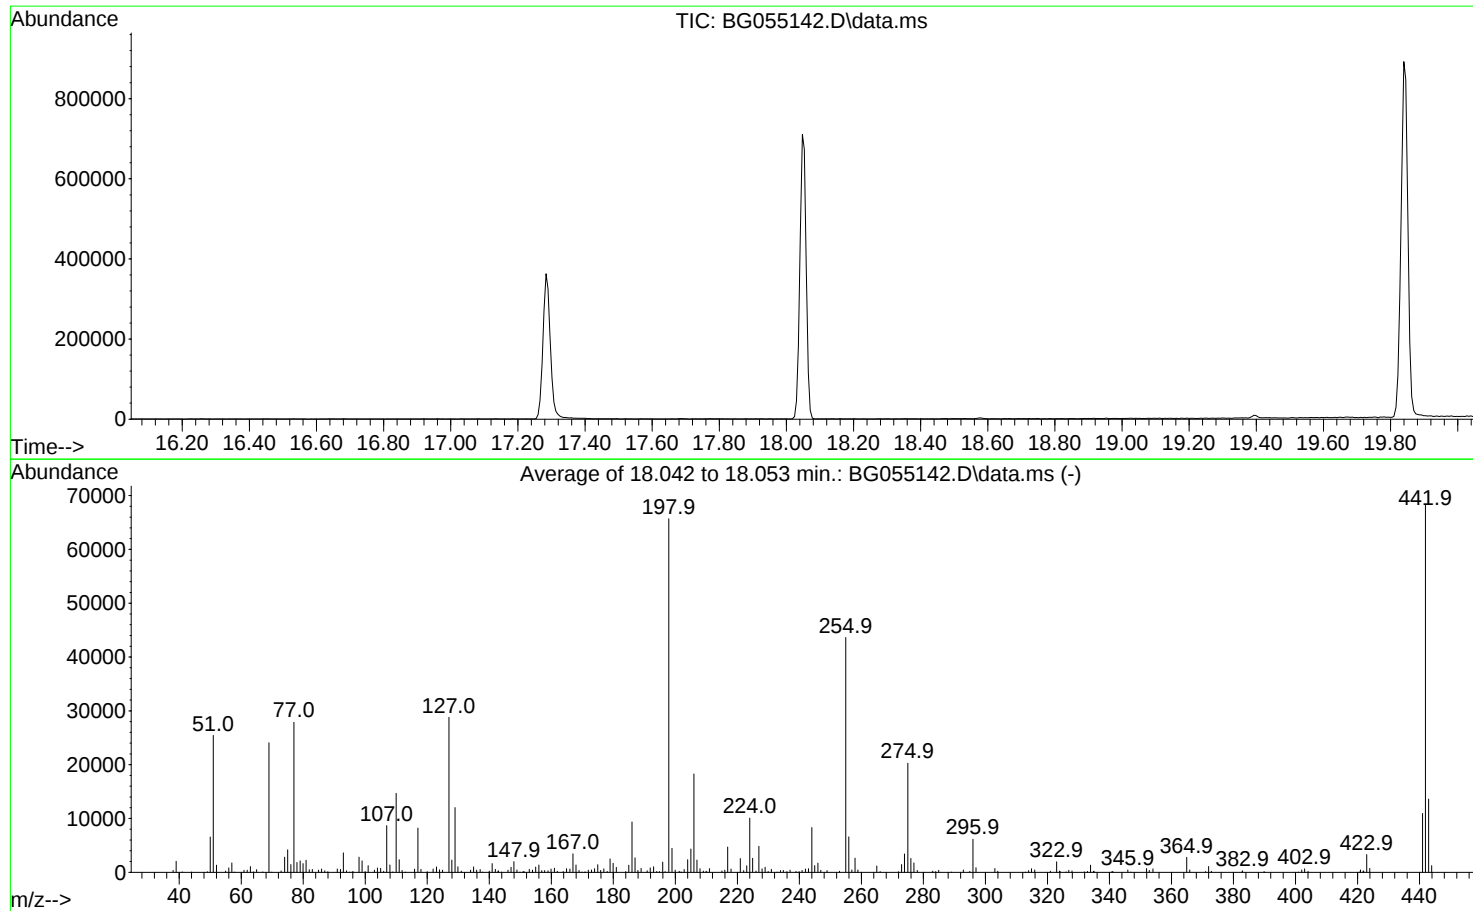




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	25440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.6	24072	PASS
70	69	0.00	2	0.2	56	PASS
127	198	10	80	43.8	28797	PASS
197	198	0.00	2	0.2	149	PASS
198	198	100	100	100.0	65685	PASS
199	198	5	9	6.8	4444	PASS
275	198	10	60	30.8	20256	PASS
365	198	1	100	4.2	2771	PASS
441	198	0.01	100	16.6	10931	PASS
442	442	50	100	100.0	68355	PASS
443	442	15	24	19.9	13611	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055142.D
Acq On : 12 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 13 06:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

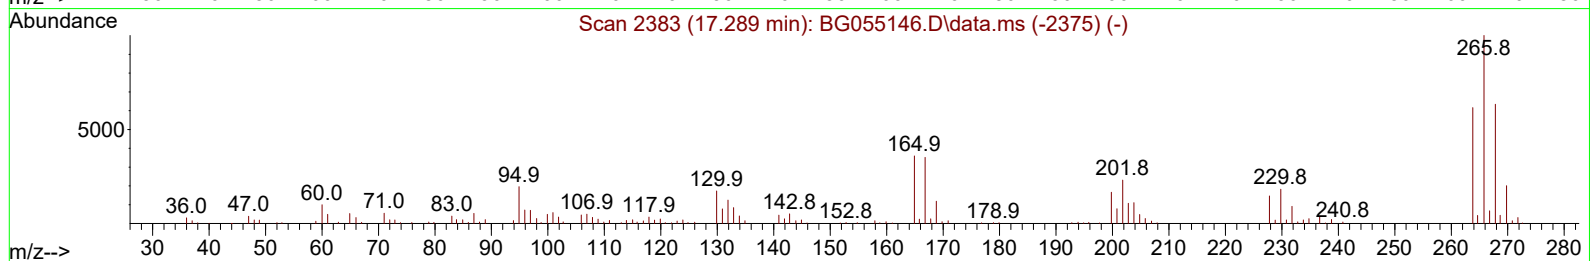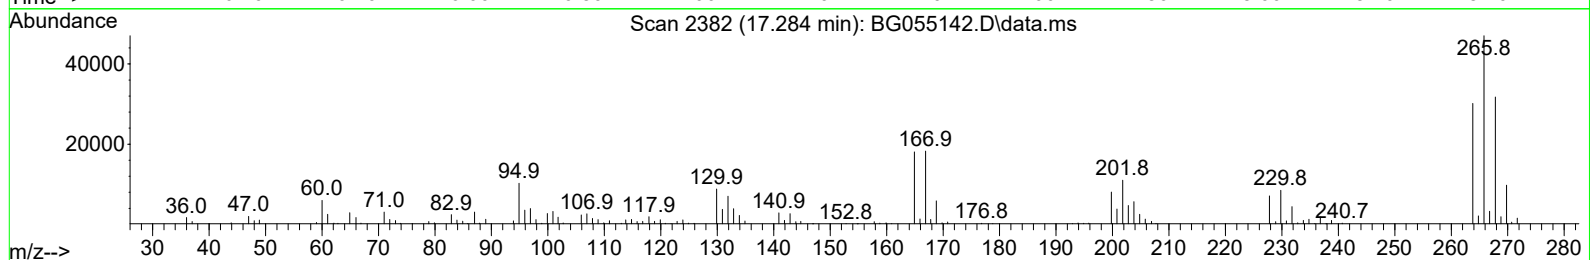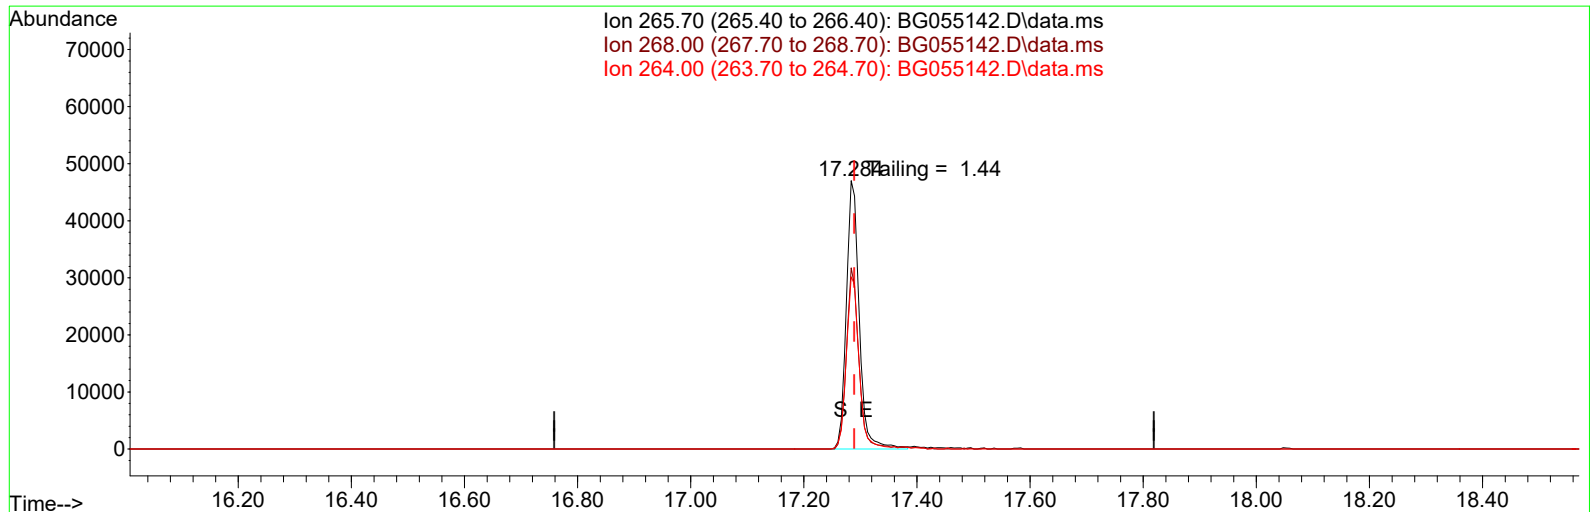

TIC: BG055142.D\data.ms

(70) Pentachlorophenol (C)

17.284min (-0.005) 21927.80 ng




response 74481

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	67.48
264.00	65.90	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055142.D
Acq On : 12 Oct 2022 15:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 13 06:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

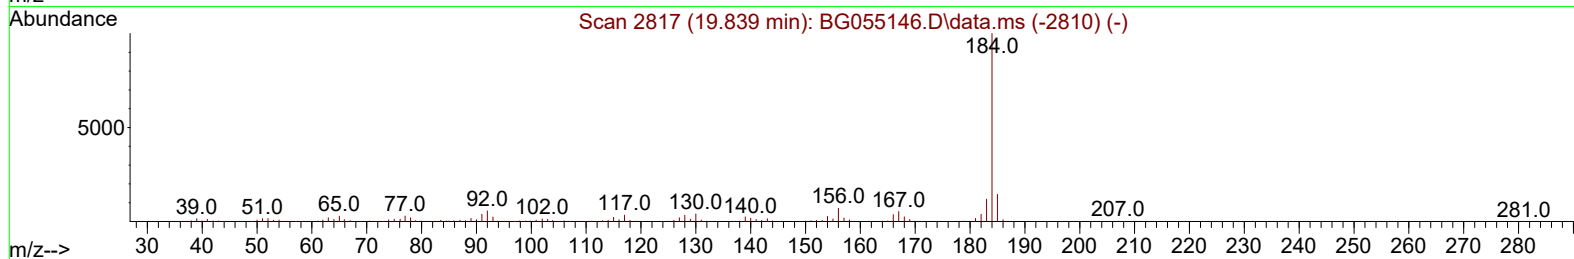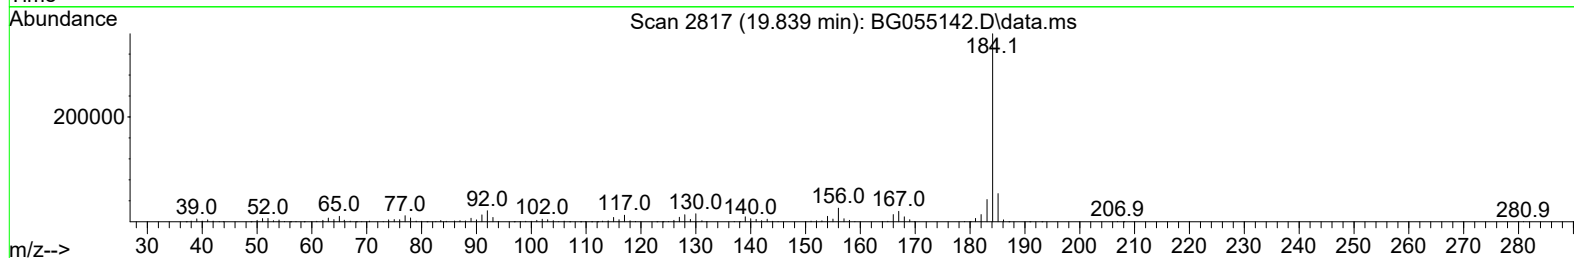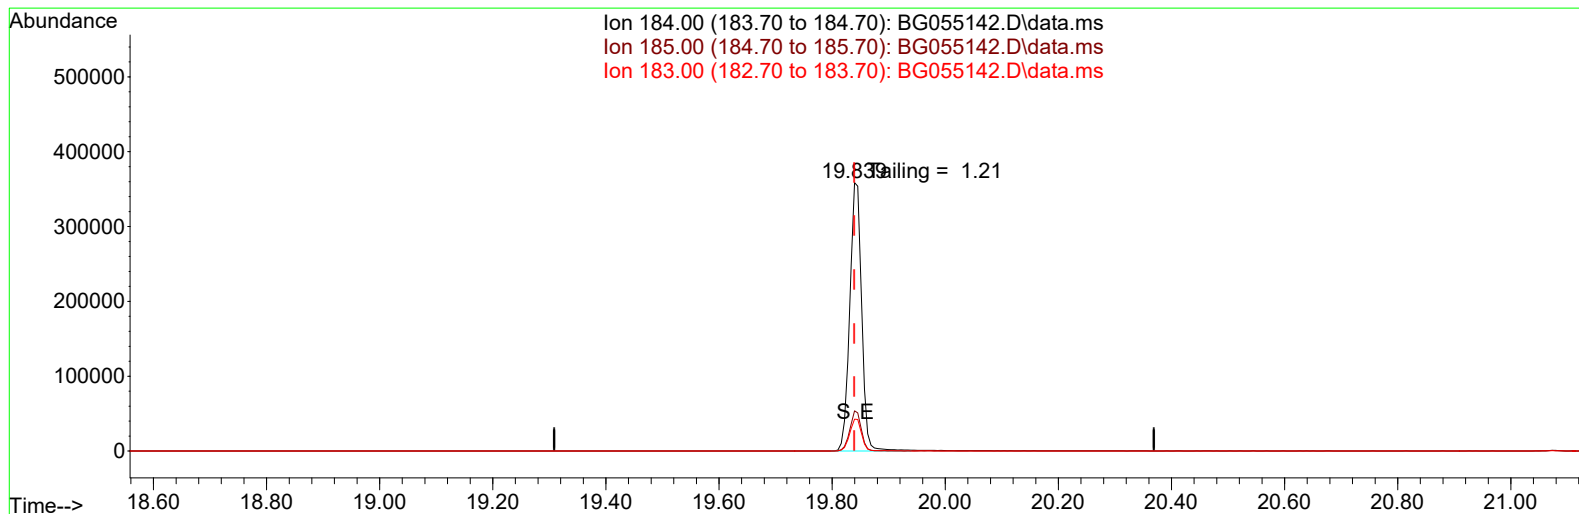

TIC: BG055142.D\data.ms

(77) Benzidine**19.839min (+ 0.001) 28871.85 ng****response 526382**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.99
183.00	11.80	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2022	BNA_G	BG055142.D
Compound Name	Response	Retention Time
DDT	235599	21.073
DDD	1918	20.68
DDE	0	20.152
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1918	237517	0.81

Instrument :
BNA_G
ClientSampleId :
DFTPP