


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
 Data File : BG055156.D
 Acq On : 13 Oct 2022 9:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 13 05:14:13 2022

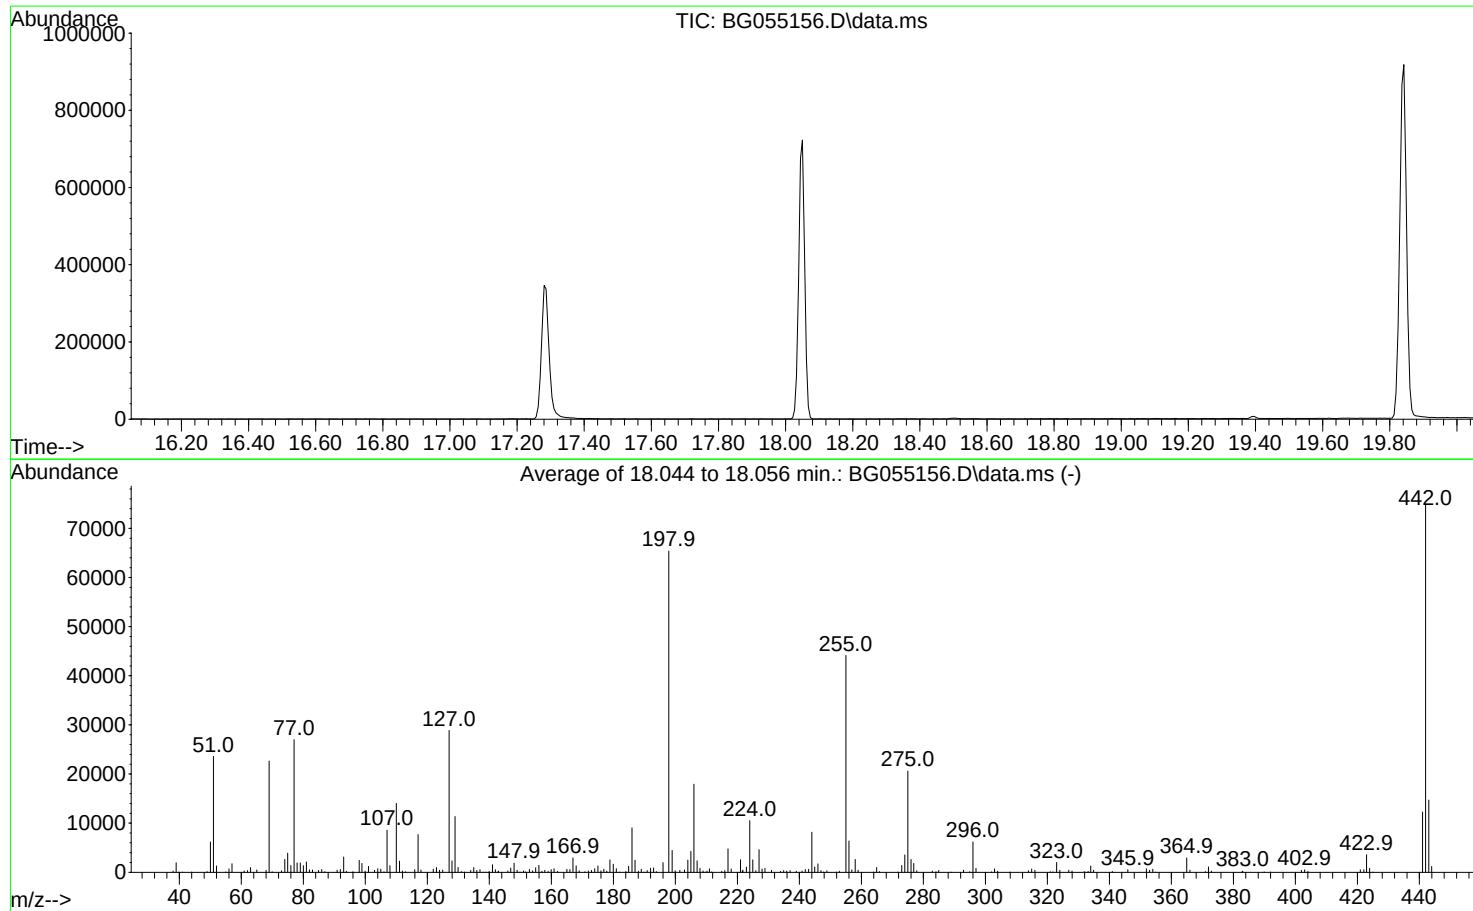




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	23591	PASS
68	69	0.00	2	1.9	423	PASS
69	198	0.00	100	34.7	22661	PASS
70	69	0.00	2	0.5	116	PASS
127	198	10	80	44.2	28883	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65368	PASS
199	198	5	9	6.8	4460	PASS
275	198	10	60	31.5	20603	PASS
365	198	1	100	4.5	2934	PASS
441	198	0.01	100	18.8	12279	PASS
442	442	50	100	100.0	74875	PASS
443	442	15	24	19.7	14722	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055156.D
Acq On : 13 Oct 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:38:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

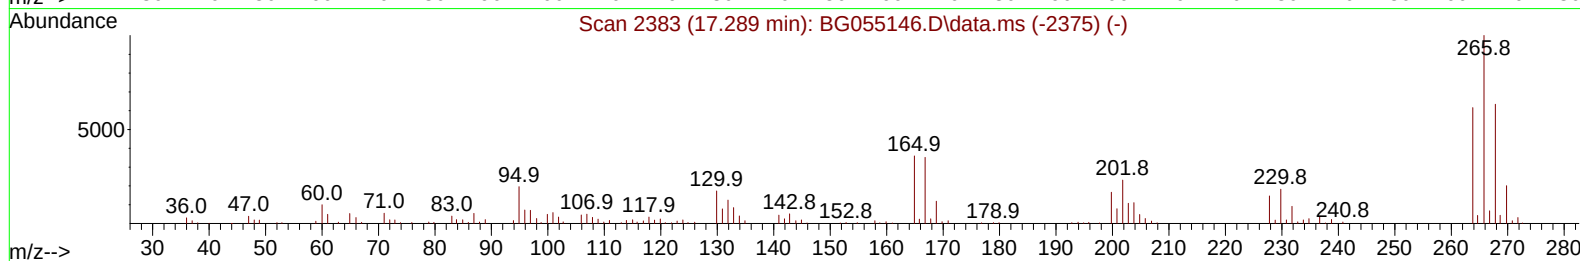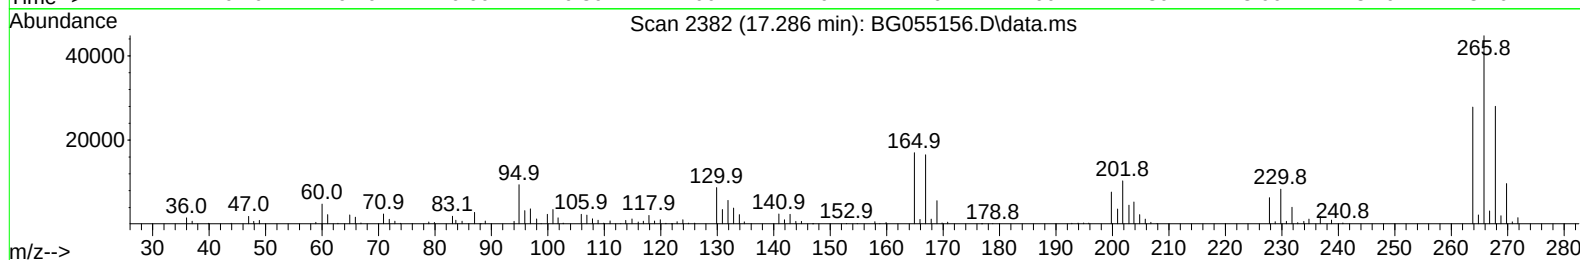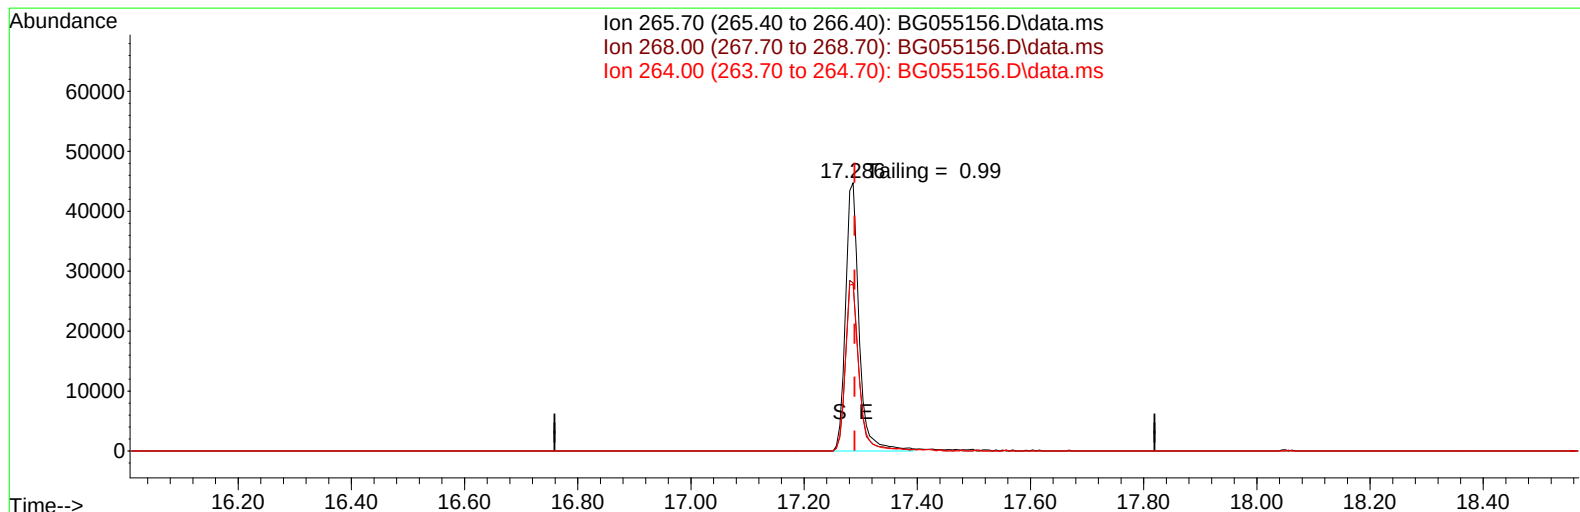

TIC: BG055156.D\data.ms

(70) Pentachlorophenol (C)

17.286min (-0.002) 31451.51 ng




response 73959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	62.60
264.00	65.90	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101322\
Data File : BG055156.D
Acq On : 13 Oct 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:38:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

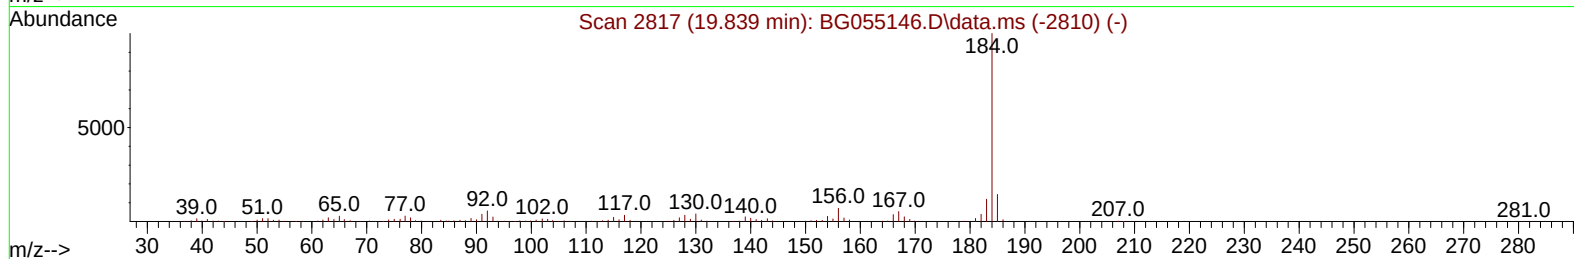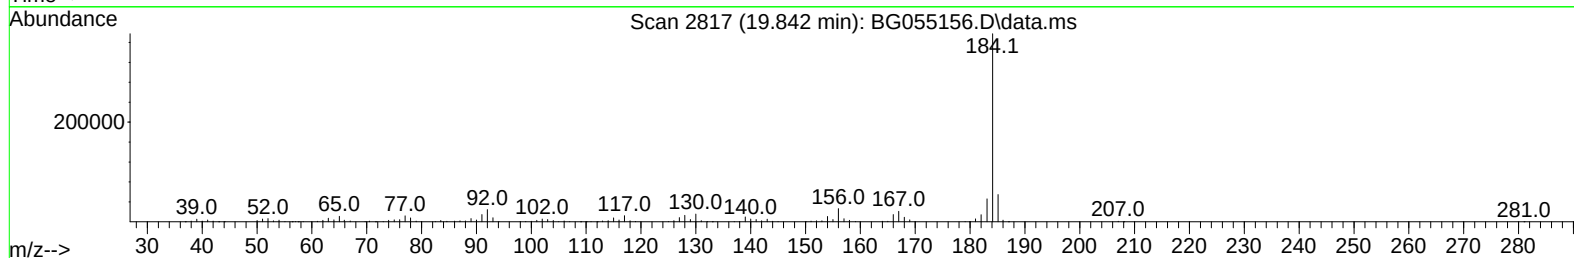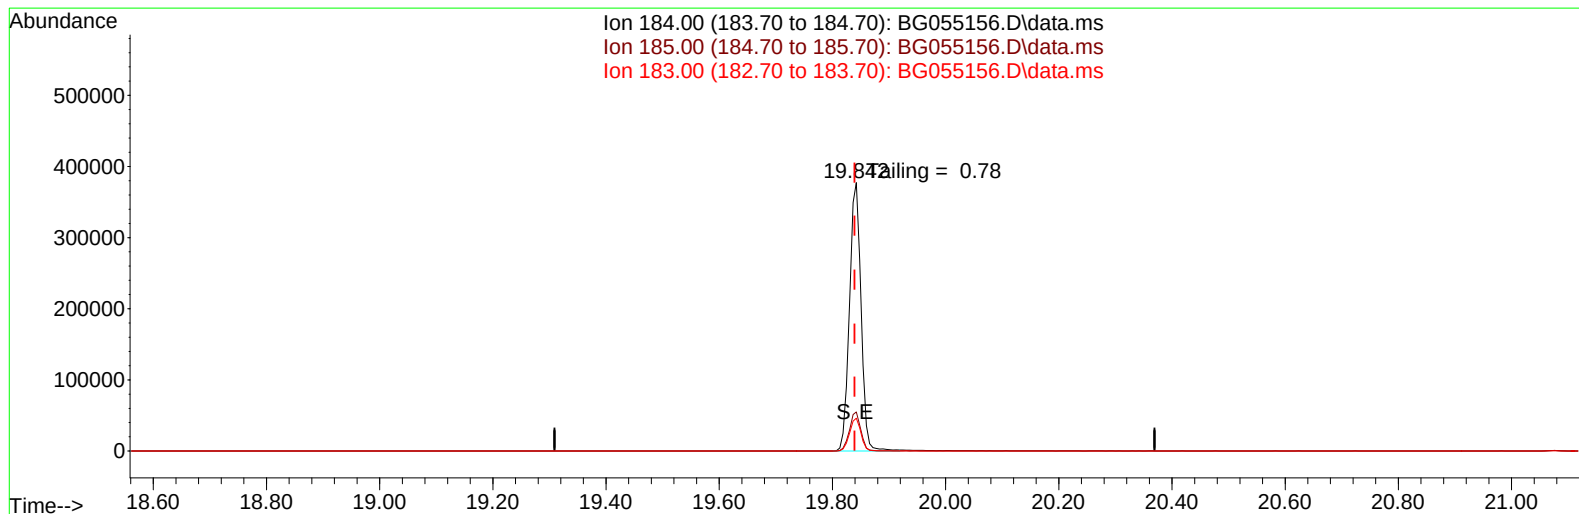

TIC: BG055156.D\data.ms

(77) Benzidine

19.842min (+ 0.003) 53426.54 ng

response 540343

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.54
183.00	11.80	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2022	BNA_G	<u>BG055156.D</u>
Compound Name	Response	Retention Time
DDT	254865	21.076
DDD	4111	20.624
DDE	0	20.152
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4111	258976	1.59

Instrument :
BNA_G
ClientSampleId :
DFTPP