

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
 Data File : BG019183.D
 Acq On : 13 Oct 2015 17:41
 Operator : UM/NP
 Sample : PB86087BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK87

Quant Time: Oct 14 03:57:54 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 03:54:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	16736	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	81299	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	57426	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	135106	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	163203	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	147953	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	1775	4.79	ng/uL	0.00
5) Phenol-d5	7.20	99	47640	33.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.35	67	30849	33.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	36249	33.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	39574	34.91	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	19957	32.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	22672	35.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	41215	32.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	59106	38.30	ng/ul	0.00
44) Dimethylphthalate-d6	14.06	166	154699	34.17	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	175260	31.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	23507	25.70	ng/ul	0.00
58) Fluorene-d10	15.65	176	133121	32.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	16864	23.01	ng/ul	0.00
71) Anthracene-d10	17.51	188	214815	33.77	ng/ul	0.00
79) Pyrene-d10	19.79	212	244702	32.37	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.69	264	274711	36.29	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.73	70	991	1.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
Data File : BG019183.D
Acq On : 13 Oct 2015 17:41
Operator : UM/NP
Sample : PB86087BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK87

Quant Time: Oct 14 03:57:54 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 03:54:50 2015
Response via : Initial Calibration

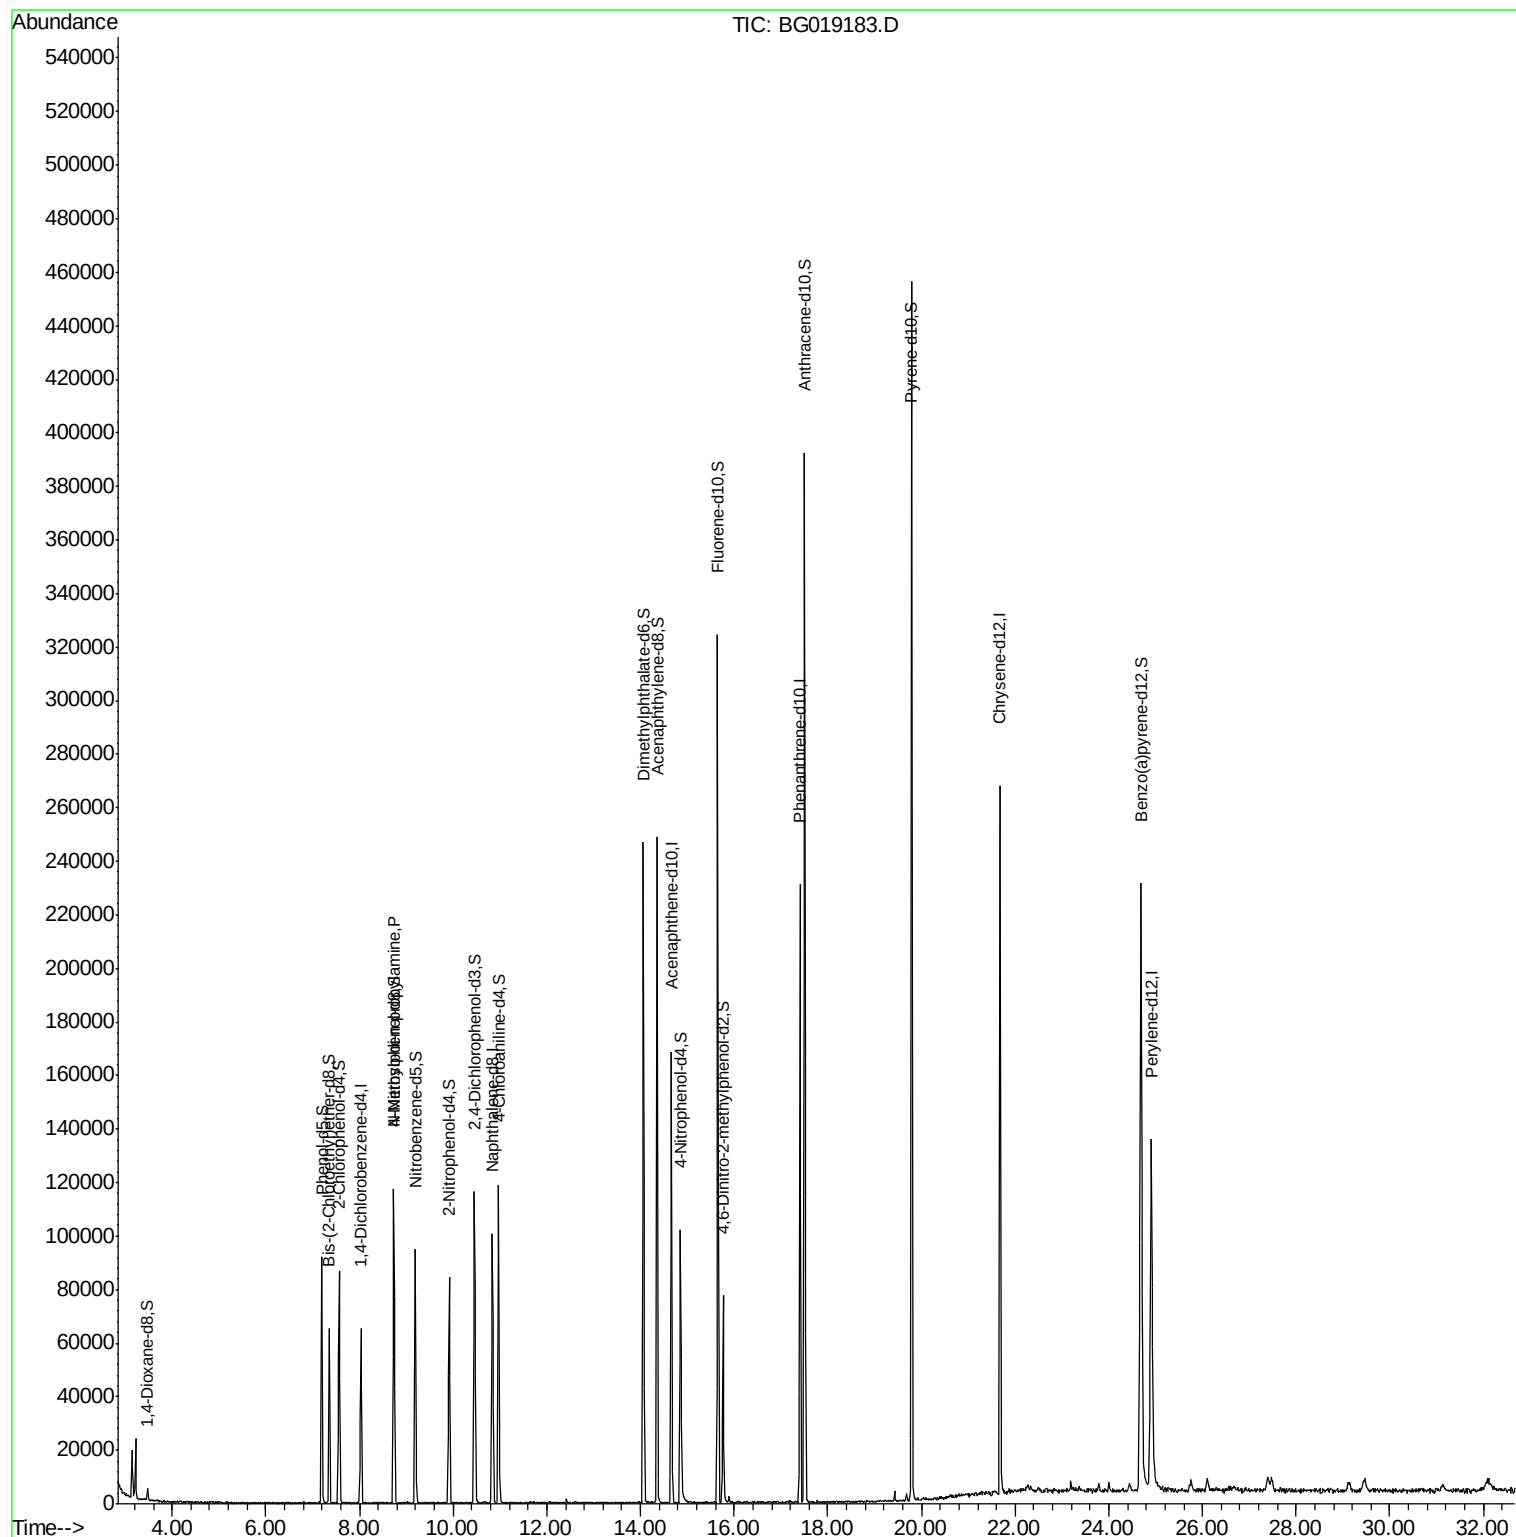

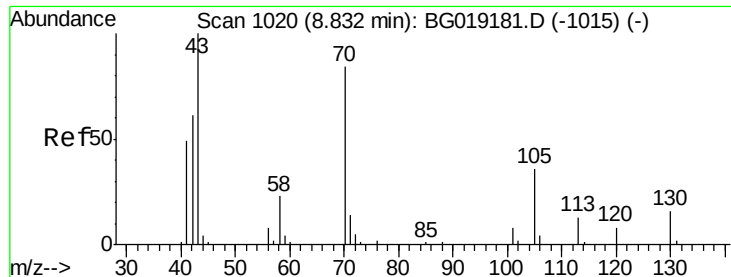

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.05 ng/ul
 RT: 8.73 min Scan# 1003
 Delta R.T. -0.10 min
 Lab File: BG019183.D
 Acq: 13 Oct 2015 17:41

Instrument :
 BNA_G
 ClientSampleId :
 SBLK87

Tot Ion: 70 Resp: 991
 Ion Ratio Lower Upper
 70 100
 42 547.0 53.6 80.4#
 101 0.0 7.9 11.9#
 130 0.0 16.5 24.7#

