

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
 Data File : BG019191.D
 Acq On : 13 Oct 2015 22:48
 Operator : UM/NP
 Sample : PB86092BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK92

Quant Time: Oct 14 04:51:32 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 04:49:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	18012	20.00	ng/ul	0.00
18) Naphthalene-d8	10.83	136	86066	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	59529	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.40	188	144555	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	170659	20.00	ng/ul	0.00
86) Perylene-d12	24.90	264	162450	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	1864	4.68	ng/uL	0.00
5) Phenol-d5	7.20	99	51270	33.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	31939	31.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	38170	32.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	43614	35.74	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	20781	31.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.91	143	24330	36.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	45901	34.26	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	62958	38.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.06	166	166490	35.47	ng/ul	0.00
47) Acenaphthylene-d8	14.35	160	187818	32.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	25177	26.55	ng/ul	0.00
58) Fluorene-d10	15.65	176	142240	33.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	20323	25.92	ng/ul	0.00
71) Anthracene-d10	17.50	188	227994	33.49	ng/ul	0.00
79) Pyrene-d10	19.79	212	258206	32.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.68	264	291037	35.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.74	70	1235	1.22	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
Data File : BG019191.D
Acq On : 13 Oct 2015 22:48
Operator : UM/NP
Sample : PB86092BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK92

Quant Time: Oct 14 04:51:32 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 04:49:14 2015
Response via : Initial Calibration

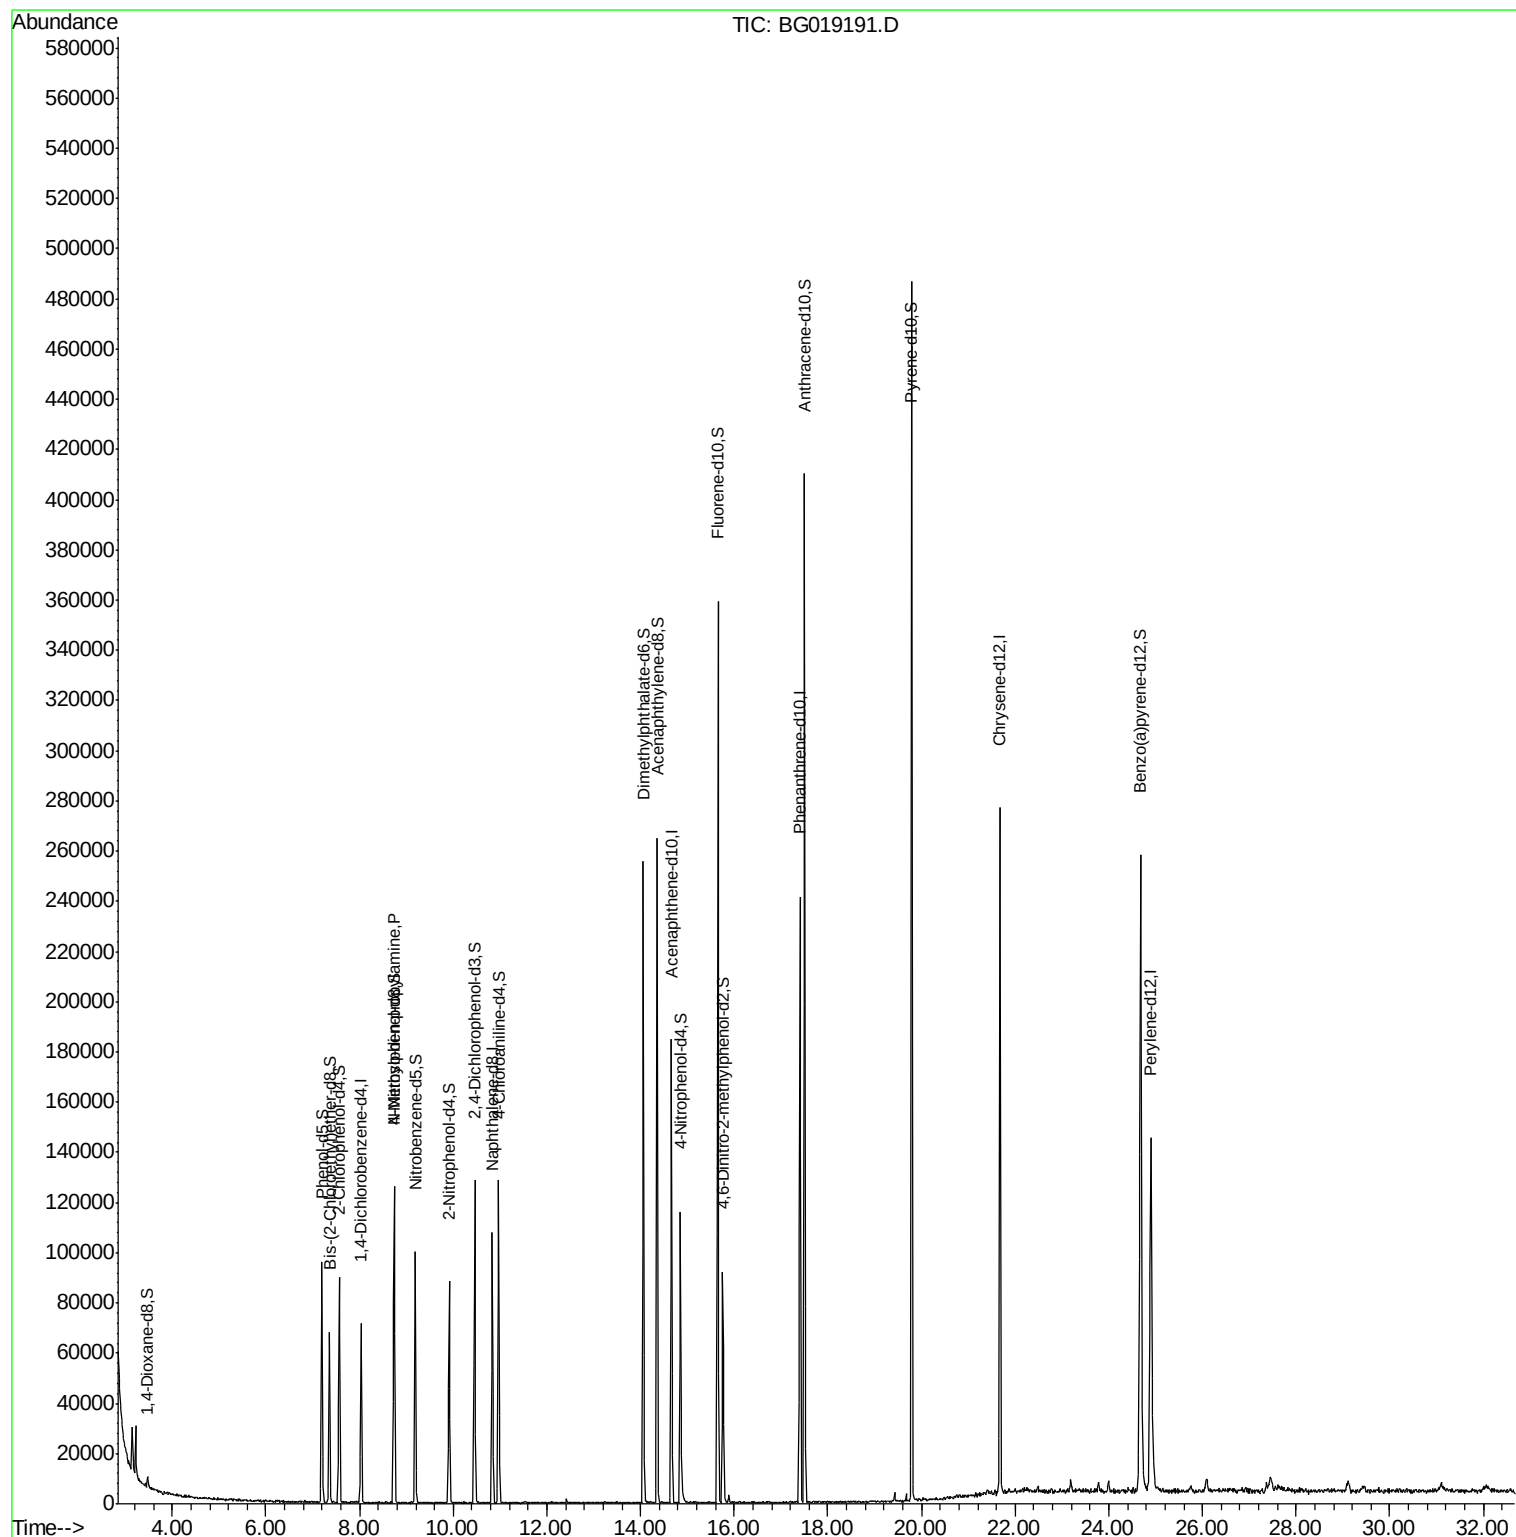

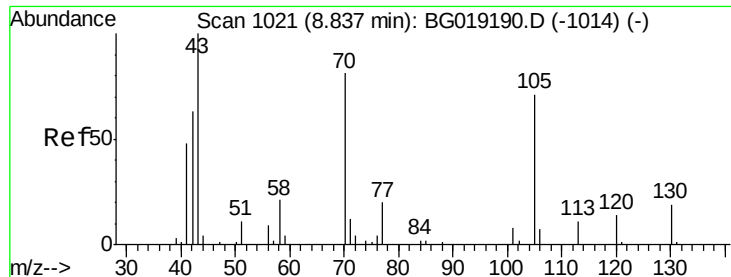

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.22 ng/ul
 RT: 8.74 min Scan# 1004
 Delta R.T. -0.10 min
 Lab File: BG019191.D
 Acq: 13 Oct 2015 22:48

Instrument :
 BNA_G
 ClientSampleId :
 SBLK92

Tot Ion:	70	Resp:	1235
Ion	Ratio	Lower	Upper
70	100		
42	422.0	53.6	80.4#
101	0.0	7.9	11.9#
130	0.0	16.5	24.7#

