

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
 Data File : BG019192.D
 Acq On : 13 Oct 2015 23:26
 Operator : UM/NP
 Sample : G3966-20
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LJ3

Quant Time: Oct 14 04:51:40 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 04:49:14 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	18397	20.00	ng/ul	0.00
18) Naphthalene-d8	10.83	136	86526	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	59160	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.40	188	141141	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	167043	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	154688	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	2127	5.22	ng/uL	0.00
5) Phenol-d5	7.19	99	50896	32.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	33738	32.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	39160	32.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	43886	35.21	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	20465	31.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.91	143	23862	35.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	45202	33.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	62678	38.16	ng/ul	0.00
44) Dimethylphthalate-d6	14.06	166	165357	35.45	ng/ul	0.00
47) Acenaphthylene-d8	14.35	160	185219	32.10	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	24700	26.21	ng/ul	0.00
58) Fluorene-d10	15.65	176	141769	33.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	18512	24.18	ng/ul	0.00
71) Anthracene-d10	17.50	188	221119	33.27	ng/ul	0.00
79) Pyrene-d10	19.79	212	253459	32.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.68	264	279252	35.28	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.74	70	1099	1.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101415\
Data File : BG019192.D
Acq On : 13 Oct 2015 23:26
Operator : UM/NP
Sample : G3966-20
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LJ3

Quant Time: Oct 14 04:51:40 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 04:49:14 2015
Response via : Initial Calibration

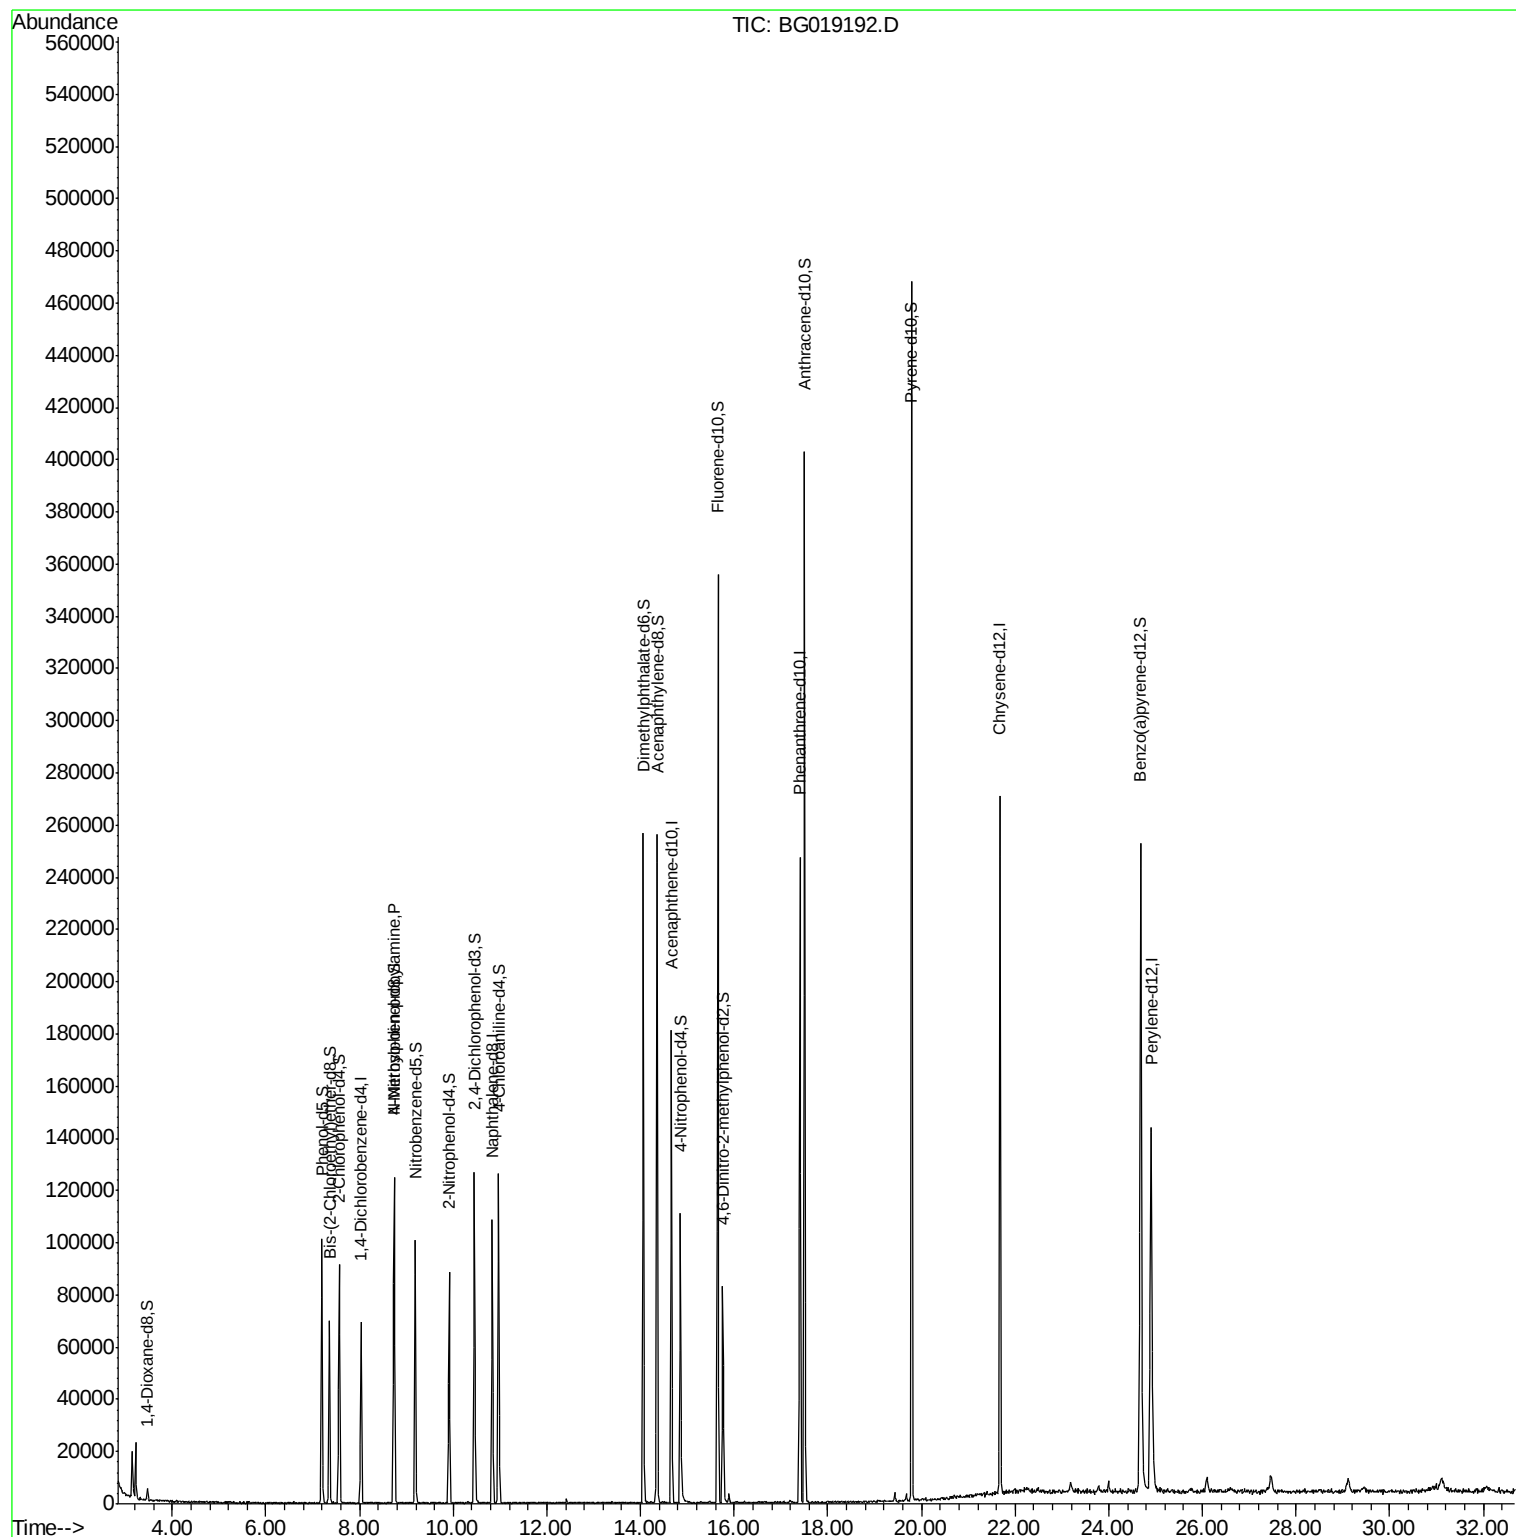

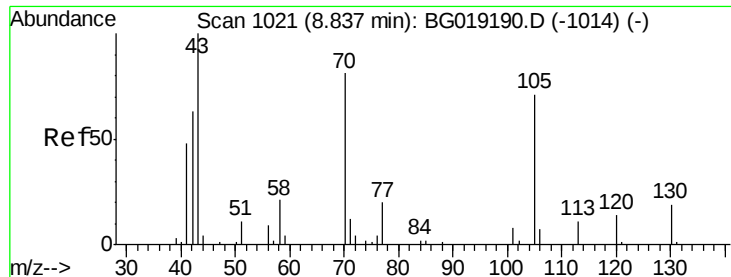

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.06 ng/ul
 RT: 8.74 min Scan# 1004
 Delta R.T. -0.10 min
 Lab File: BG019192.D
 Acq: 13 Oct 2015 23:26

Instrument :
 BNA_G
 ClientSampleId :
 E5LJ3

Tot Ion:	70	Resp:	1099
Ion	Ratio	Lower	Upper
70	100		
42	466.1	53.6	80.4#
101	0.0	7.9	11.9#
130	0.0	16.5	24.7#

