

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101420\
 Data File : BG046903.D
 Acq On : 14 Oct 2020 21:49
 Operator : CG/JU
 Sample : L4209-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 15 00:39:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 15 00:34:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	63408	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	254700	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	193865	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	491956	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	528377	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	497406	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.52	96	7457	5.77	ng/uL	0.00
5) Phenol-d5	7.25	99	73034	13.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	121197	36.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	109448	27.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	67281	15.85	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	82227	43.13	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	89693	46.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	148239	32.52	ng/ul	0.00
29) 4-Chloroaniline-d4	11.04	131	72031	13.30	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	648098	43.75	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	401054	22.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	53632	21.24	ng/ul	0.00
58) Fluorene-d10	15.71	176	555089	40.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	134523	54.73	ng/ul	0.00
71) Anthracene-d10	17.57	188	673127	29.82	ng/ul	0.00
79) Pyrene-d10	19.84	212	933904	34.06	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	915388	34.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.17	163	34190	2.281	ng/ul#	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101420\
Data File : BG046903.D
Acq On : 14 Oct 2020 21:49
Operator : CG/JU
Sample : L4209-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 15 00:39:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 15 00:34:52 2020
Response via : Initial Calibration

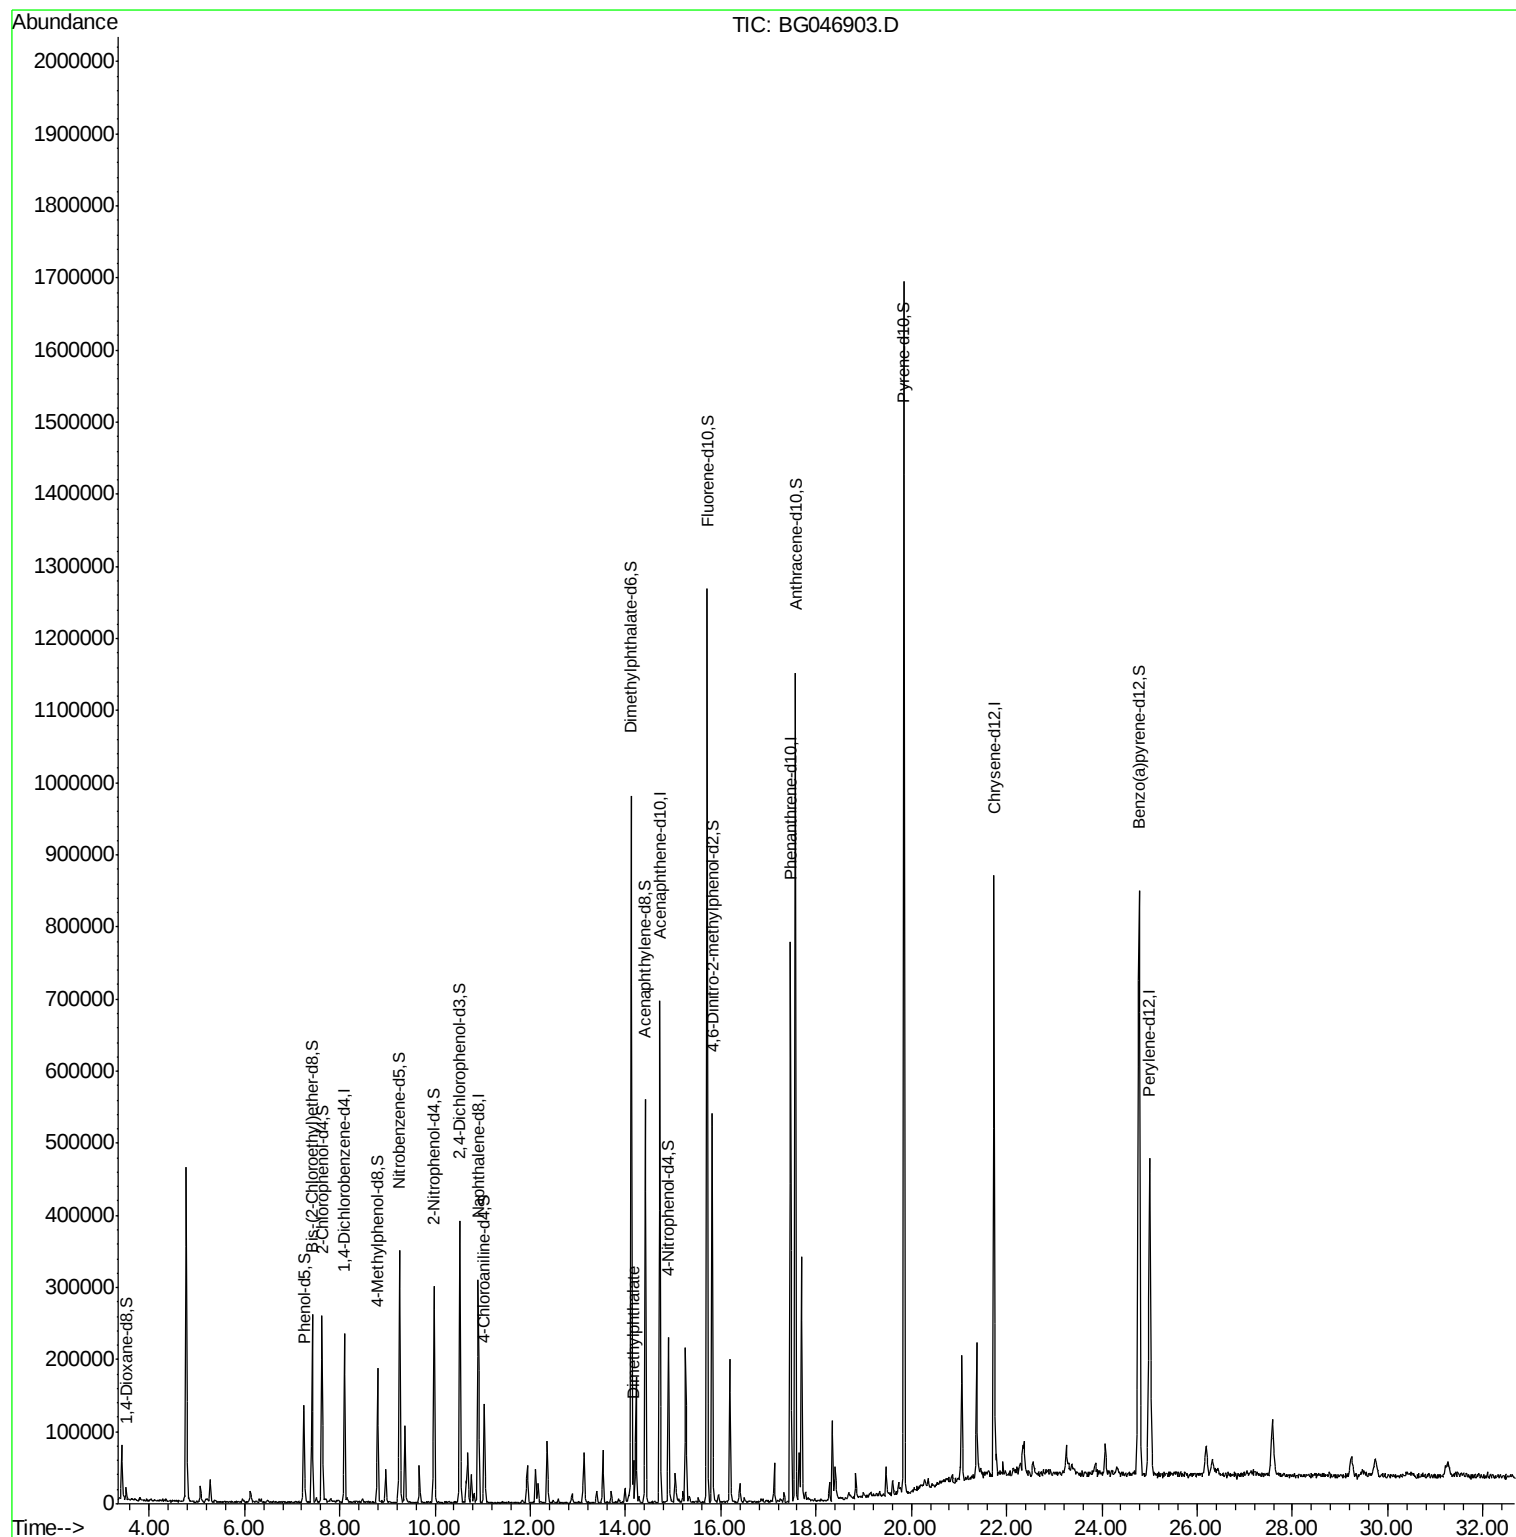

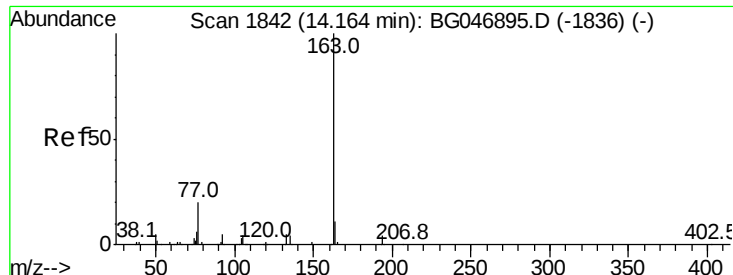

#45

Dimethylphthalate

Concen: 2.281 ng/ul

RT: 14.17 min Scan# 1843

Delta R.T. 0.00 min

Lab File: BG046903.D

Acq: 14 Oct 2020 21:49

Instrument :

BNA_G

ClientSampleId :

Tot Ion:163 Resp: 34190

Ion Ratio Lower Upper

163 100

194 8.9 3.6 5.4#

164 11.0 7.4 11.0

