

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101420\
 Data File : BG046896.D
 Acq On : 14 Oct 2020 17:06
 Operator : CG/JU
 Sample : L4359-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7N5

Manual Integrations
 APPROVED

mohammad
 10/15/2020 8:20:04 AM

Quant Time: Oct 14 17:55:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 14 13:03:47 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	60159	20.00	ng/ul	0.00
18) Naphthalene-d8	10.91	136	235896	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.72	164	168987	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	416619	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	485924	20.00	ng/ul	0.00
86) Perylene-d12	25.00	264	479738	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.52	96	6176	5.04	ng/uL	0.00
5) Phenol-d5	7.24	99	26076	5.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.42	67	52728	16.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.62	132	62003	16.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.79	113	44791	11.12	ng/ul	0.00
19) Nitrobenzene-d5	9.26	128	35455	20.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.98	143	40933	22.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.52	165	85445	20.24	ng/ul	0.00
29) 4-Chloroaniline-d4	11.03	131	96209	19.18	ng/ul	0.00
44) Dimethylphthalate-d6	14.12	166	296746	22.98	ng/ul	0.00
47) Acenaphthylene-d8	14.42	160	319352	20.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	11913	5.41	ng/ul	0.00
58) Fluorene-d10	15.71	176	243903	20.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	44198	21.23	ng/ul	0.00
71) Anthracene-d10	17.57	188	409252m	21.41	ng/ul	0.00
79) Pyrene-d10	19.84	212	534037	21.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	549693	21.26	ng/ul	0.00

Target Compounds					Ovalue	
2) 1,4-Dioxane	3.55	88	9921	6.315	ng/uL#	84
6) Phenol	7.27	94	6582	1.220	ng/ul	92
45) Dimethylphthalate	14.16	163	14693	1.124	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG101420\
Data File : BG046896.D
Acq On : 14 Oct 2020 17:06
Operator : CG/JU
Sample : L4359-07
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB7N5

Quant Time: Oct 14 17:55:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 14 13:03:47 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
10/15/2020 8:20:04 AM

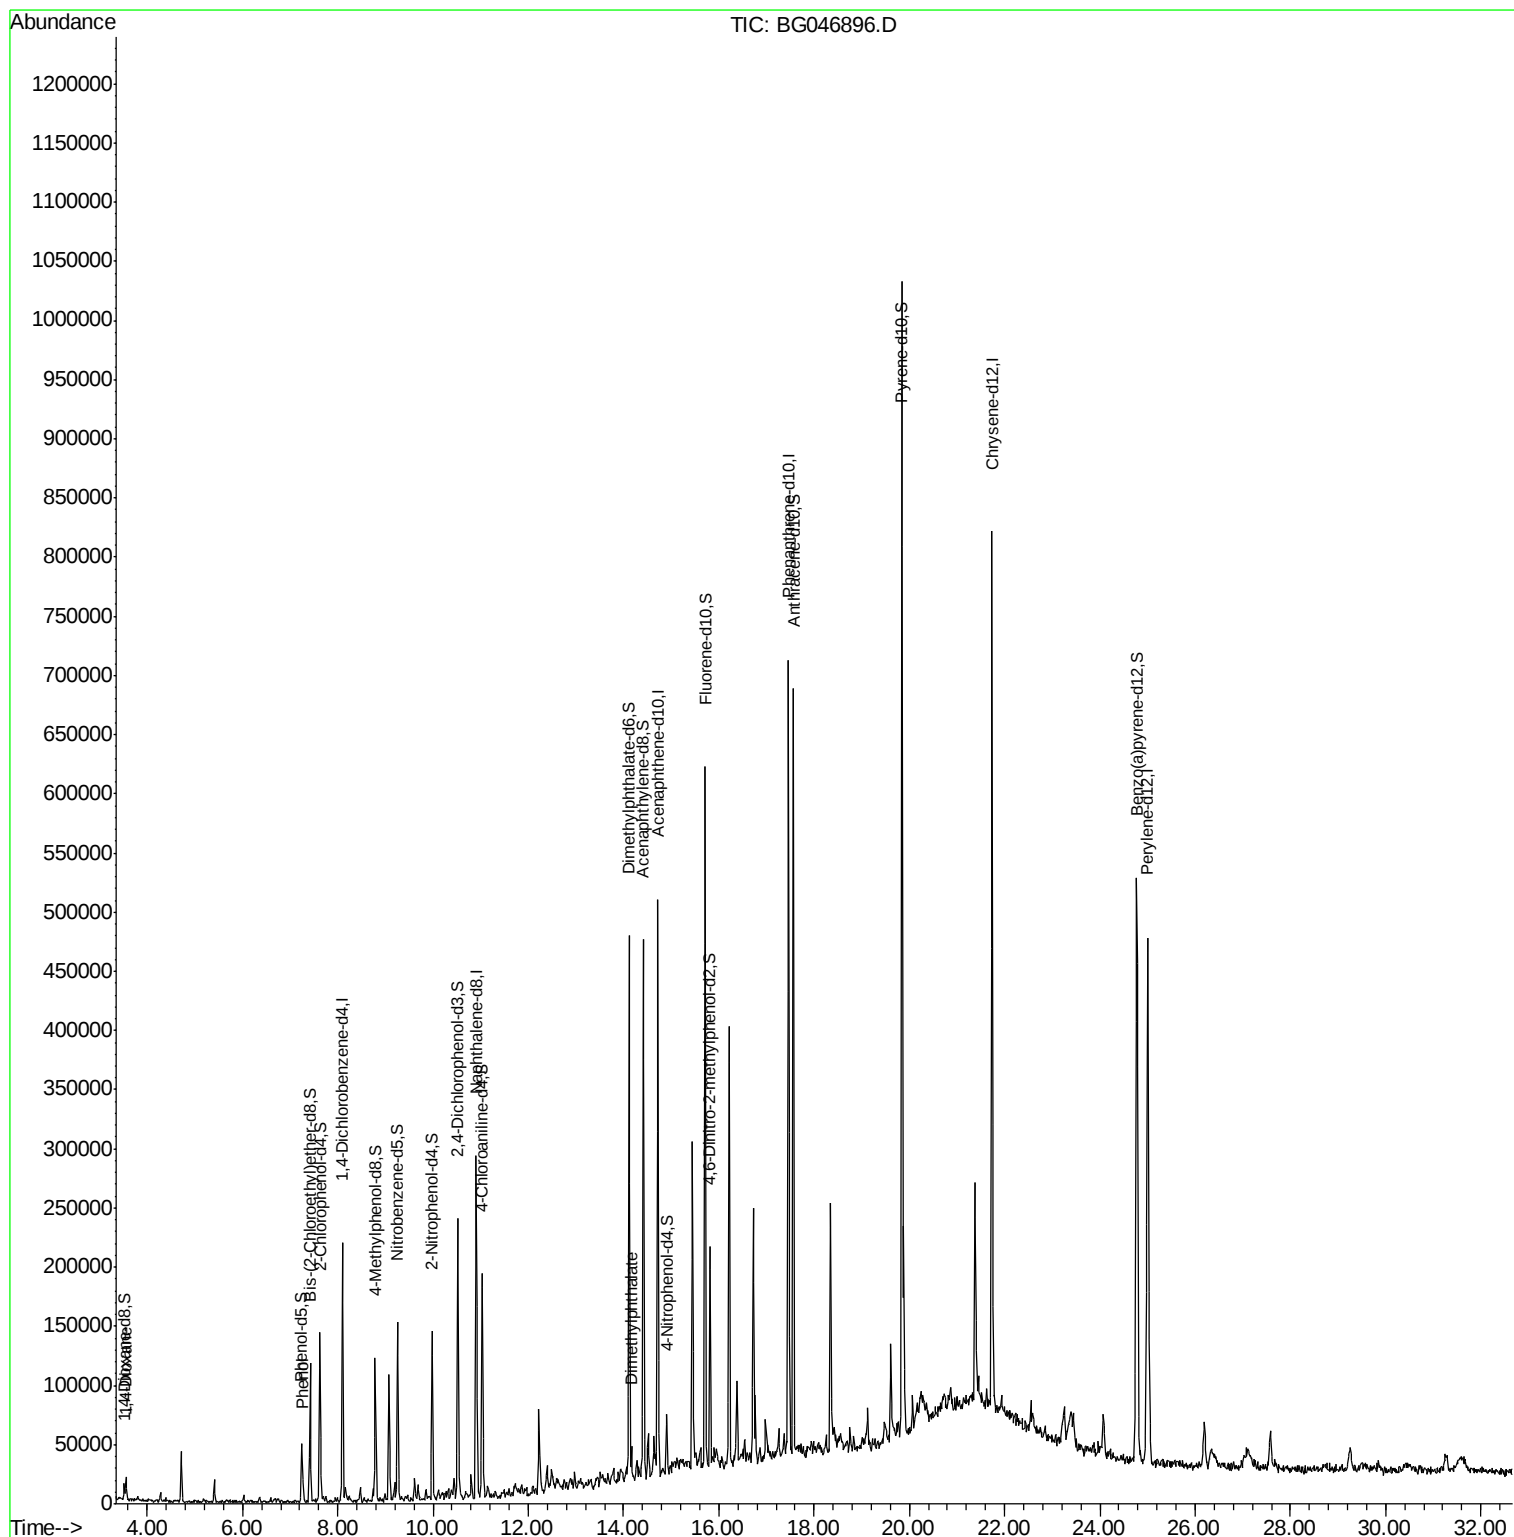

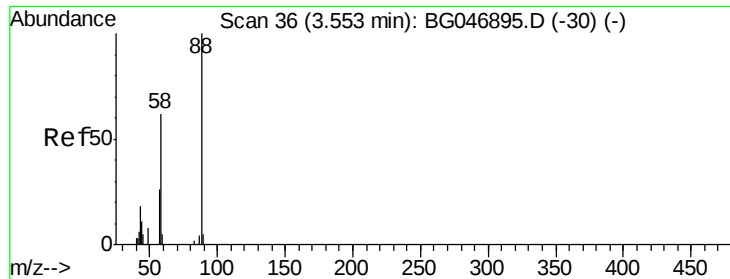

#2

1,4-Dioxane

Concen: 6.315 ng/uL

RT: 3.55 min Scan# 36

Delta R.T. -0.00 min

Lab File: BG046896.D

Acq: 14 Oct 2020 17:06

Instrument :

BNA_G


ClientSampleId :

CB7N5




Tot Ion:	88	Resp:	9921
Ion	Ratio	Lower	Upper
88	100		
43	29.1	22.3	33.5
58	60.0	62.2	93.2#

Manual Integrations
APPROVED

mohammad
10/15/2020 8:20:04 AM

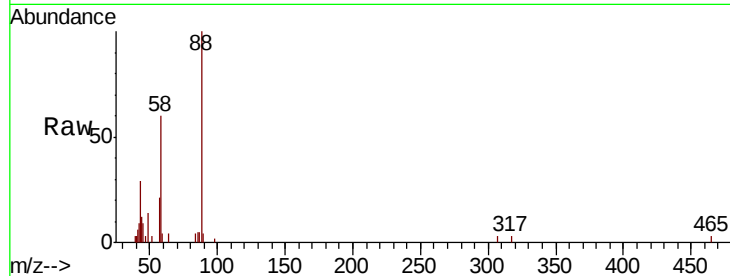

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 43.00 (42.70 to 43.70): BGC
Ion 58.00 (57.70 to 58.70): BGC

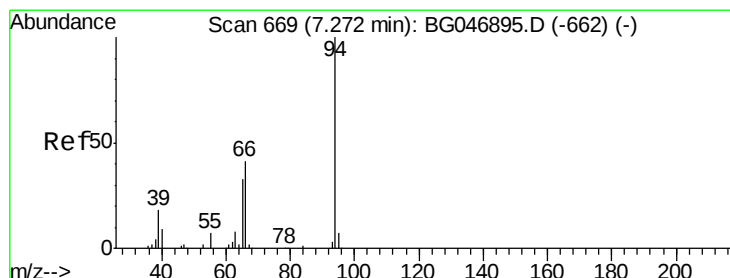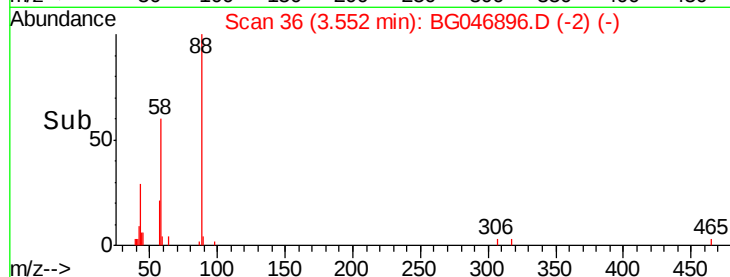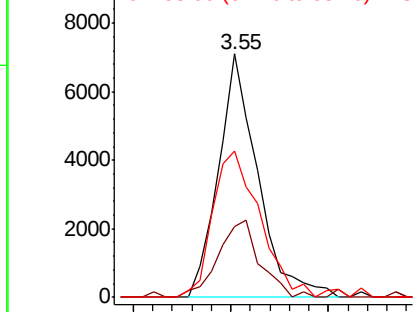

#6

Phenol

Concen: 1.220 ng/uL


RT: 7.27 min Scan# 668

Delta R.T. -0.01 min



Lab File: BG046896.D


Acq: 14 Oct 2020 17:06

Tgt Ion:	94	Resp:	6582
Ion	Ratio	Lower	Upper
94	100		
65	26.7	25.9	38.9
66	41.0	36.6	54.8

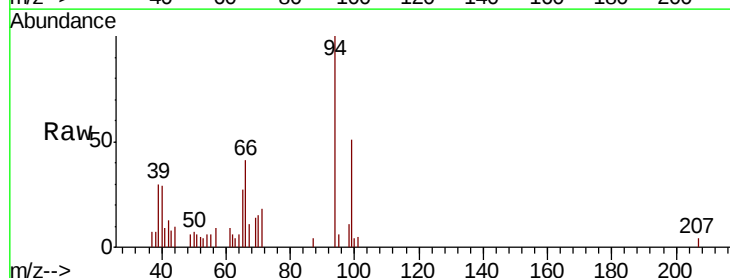

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

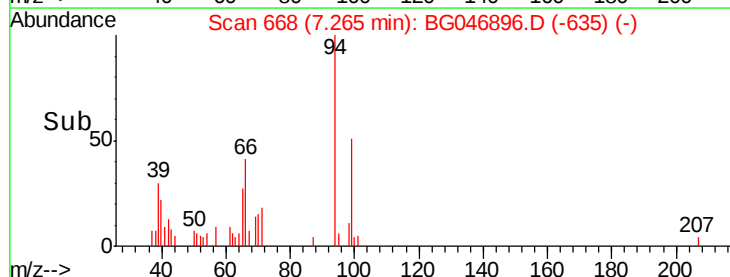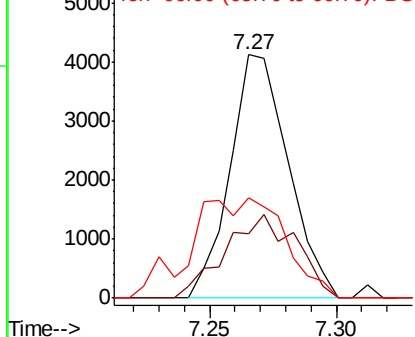

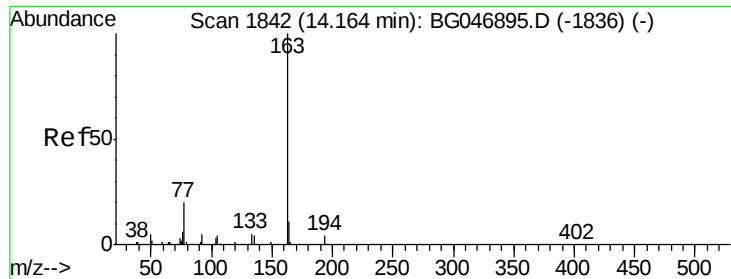

#45
 Dimethylphthalate
 Concen: 1.124 ng/ul
 RT: 14.16 min Scan# 1842
 Delta R.T. -0.00 min
 Lab File: BG046896.D
 Acq: 14 Oct 2020 17:06

Instrument :
 BNA_G
 ClientSampleId :
 CB7N5

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.1	3.6	5.4#
164	11.1	7.4	11.0#

Manual Integrations
 APPROVED

mohammad
 10/15/2020 8:20:04 AM

