
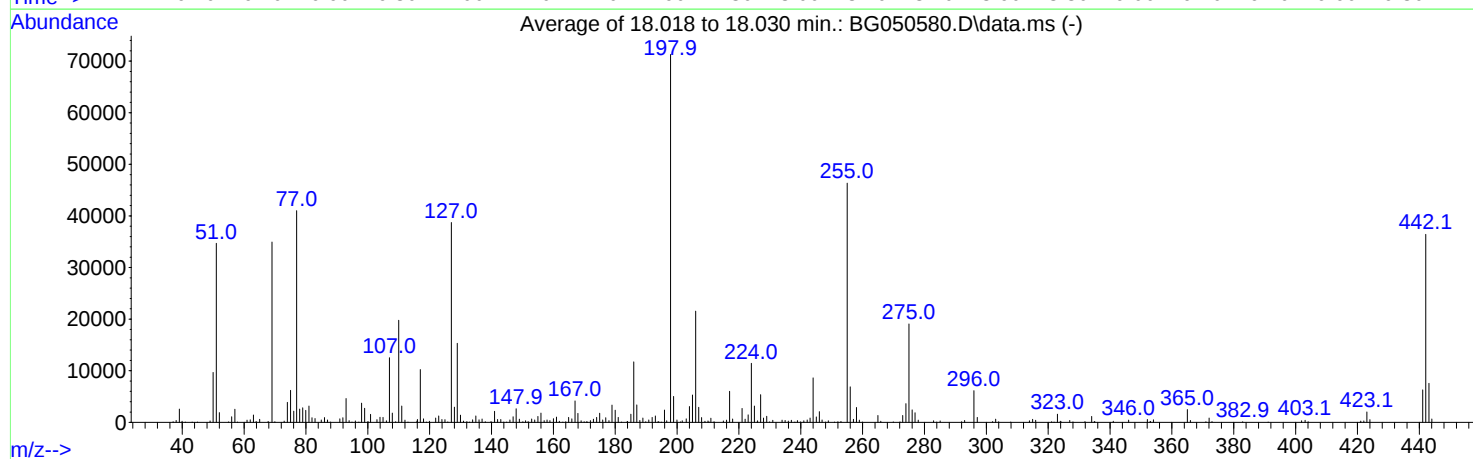


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101421\
 Data File : BG050580.D
 Acq On : 14 Oct 2021 9:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

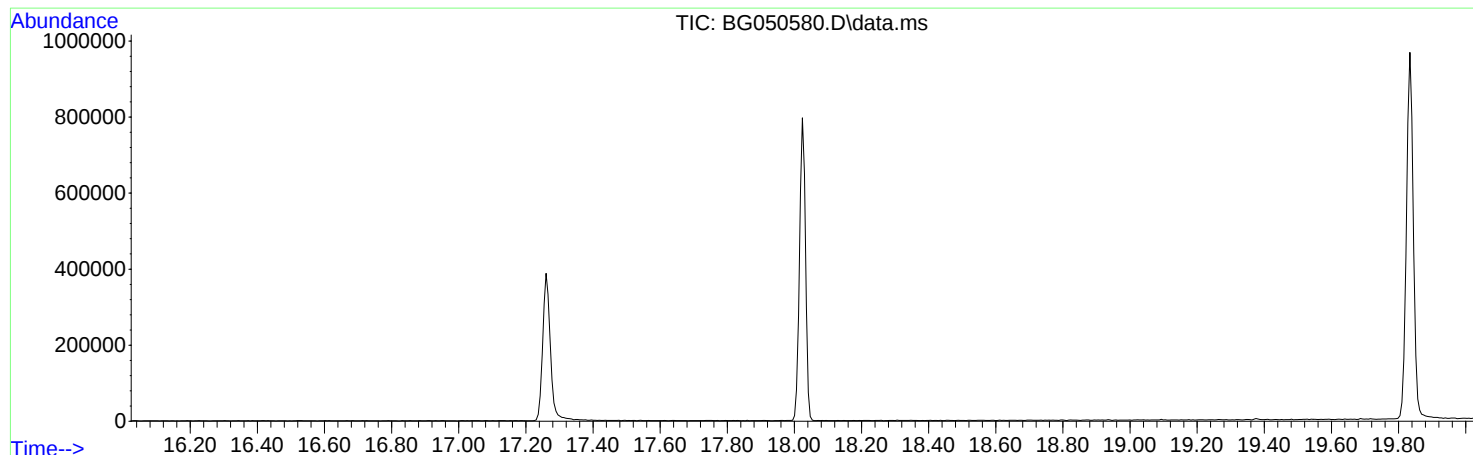




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	34683	PASS
68	69	0.00	2	0.6	193	PASS
69	198	0.00	100	49.0	34949	PASS
70	69	0.00	2	0.4	142	PASS
127	198	10	80	54.3	38717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71272	PASS
199	198	5	9	7.1	5026	PASS
275	198	10	60	26.7	19053	PASS
365	198	1	100	3.5	2489	PASS
441	198	0.01	100	8.8	6294	PASS
442	442	50	100	100.0	36429	PASS
443	442	15	24	20.8	7568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101421\
Data File : BG050580.D
Acq On : 14 Oct 2021 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 15 06:31:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

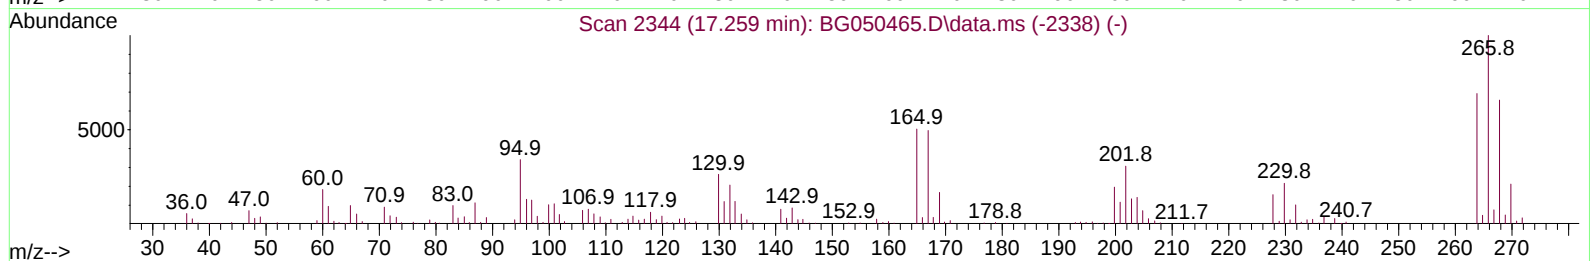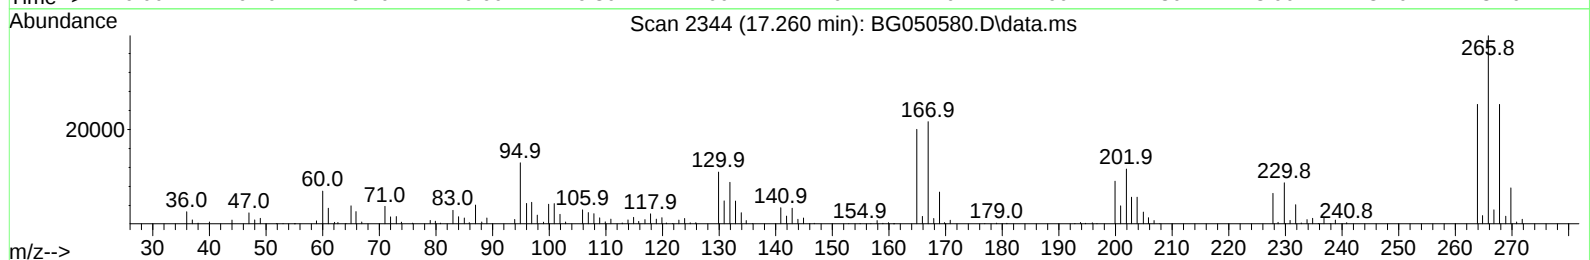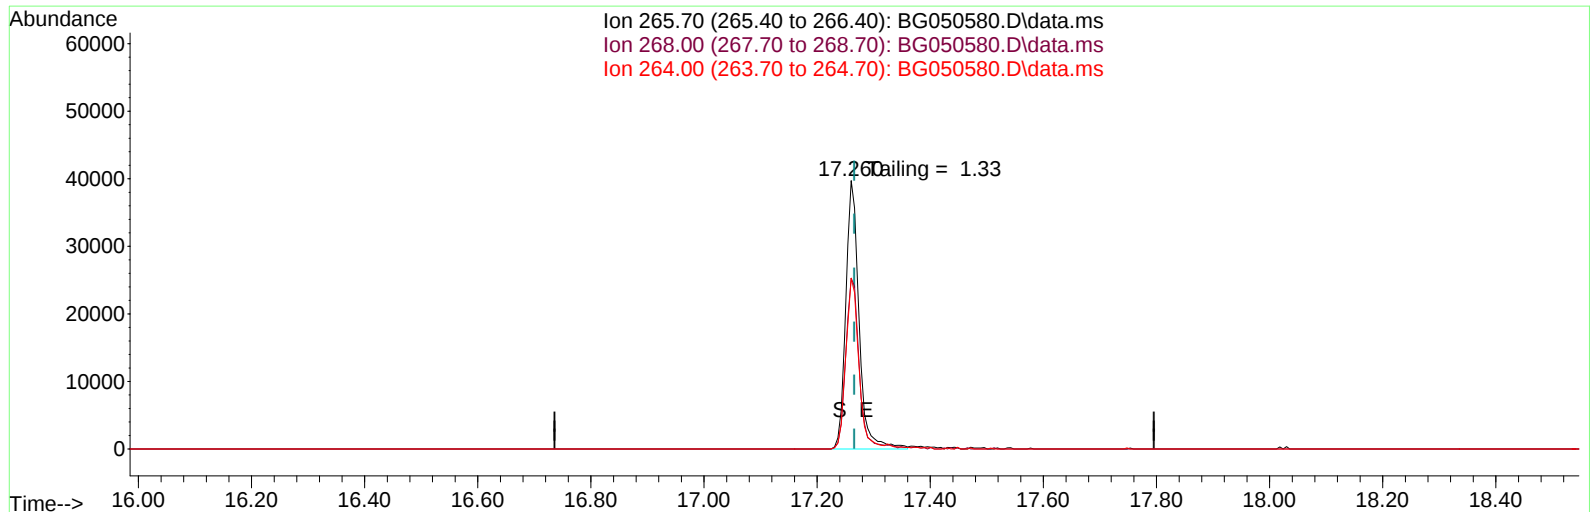

TIC: BG050580.D\data.ms

(70) Pentachlorophenol (C)

17.260min (-0.005) 23303.62 ng




response 64982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.59
264.00	61.30	63.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101421\
Data File : BG050580.D
Acq On : 14 Oct 2021 9:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 15 06:31:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

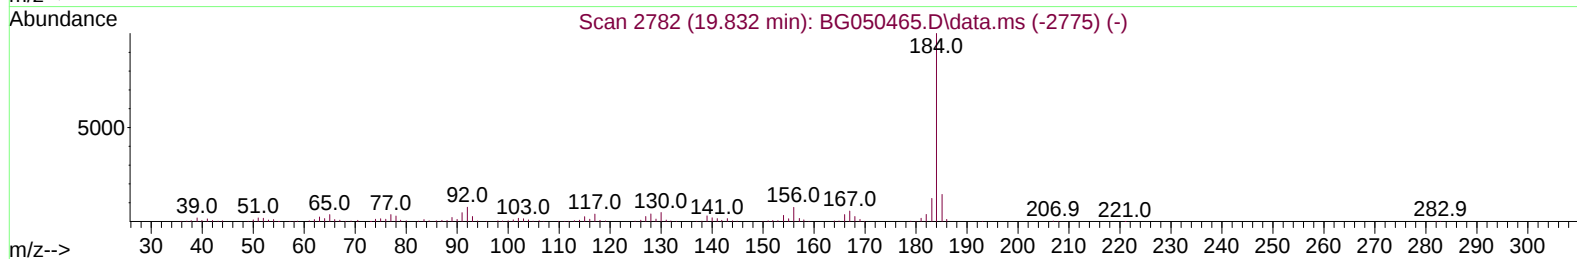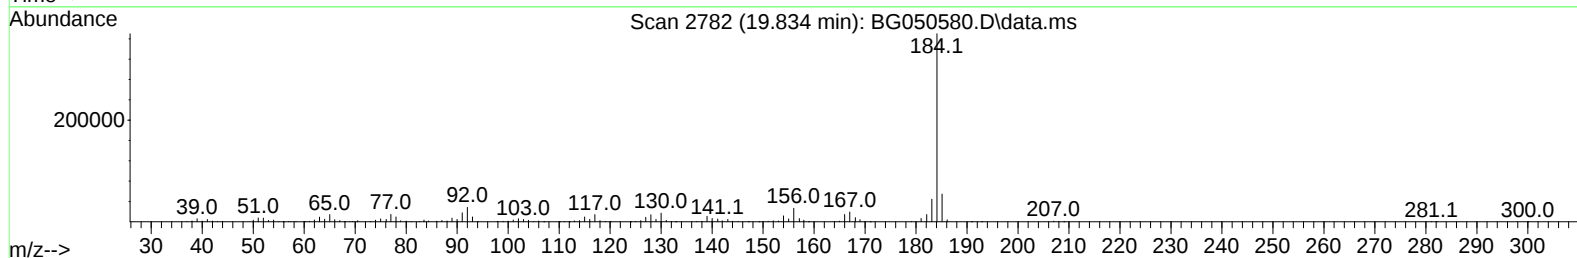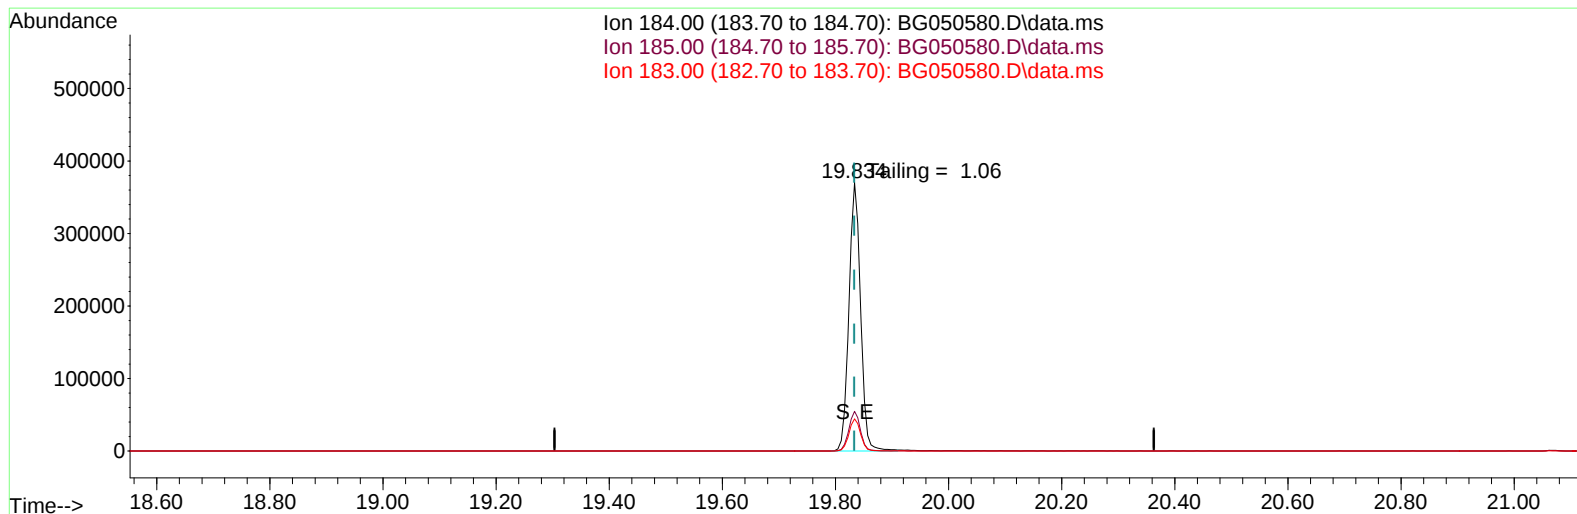

TIC: BG050580.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 0.00 ng

response 532473

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.78
183.00	11.70	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/14/2021	BNA_G	BG050580.D
Compound Name	Response	Retention Time
DDT	237353	21.067
DDD	4102	20.621
DDE	655	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4757	242110	1.96

Instrument :
BNA_G
ClientSampleId :
DFTPP