


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101422\
Data File : BG055173.D
Acq On : 14 Oct 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 13 05:14:13 2022

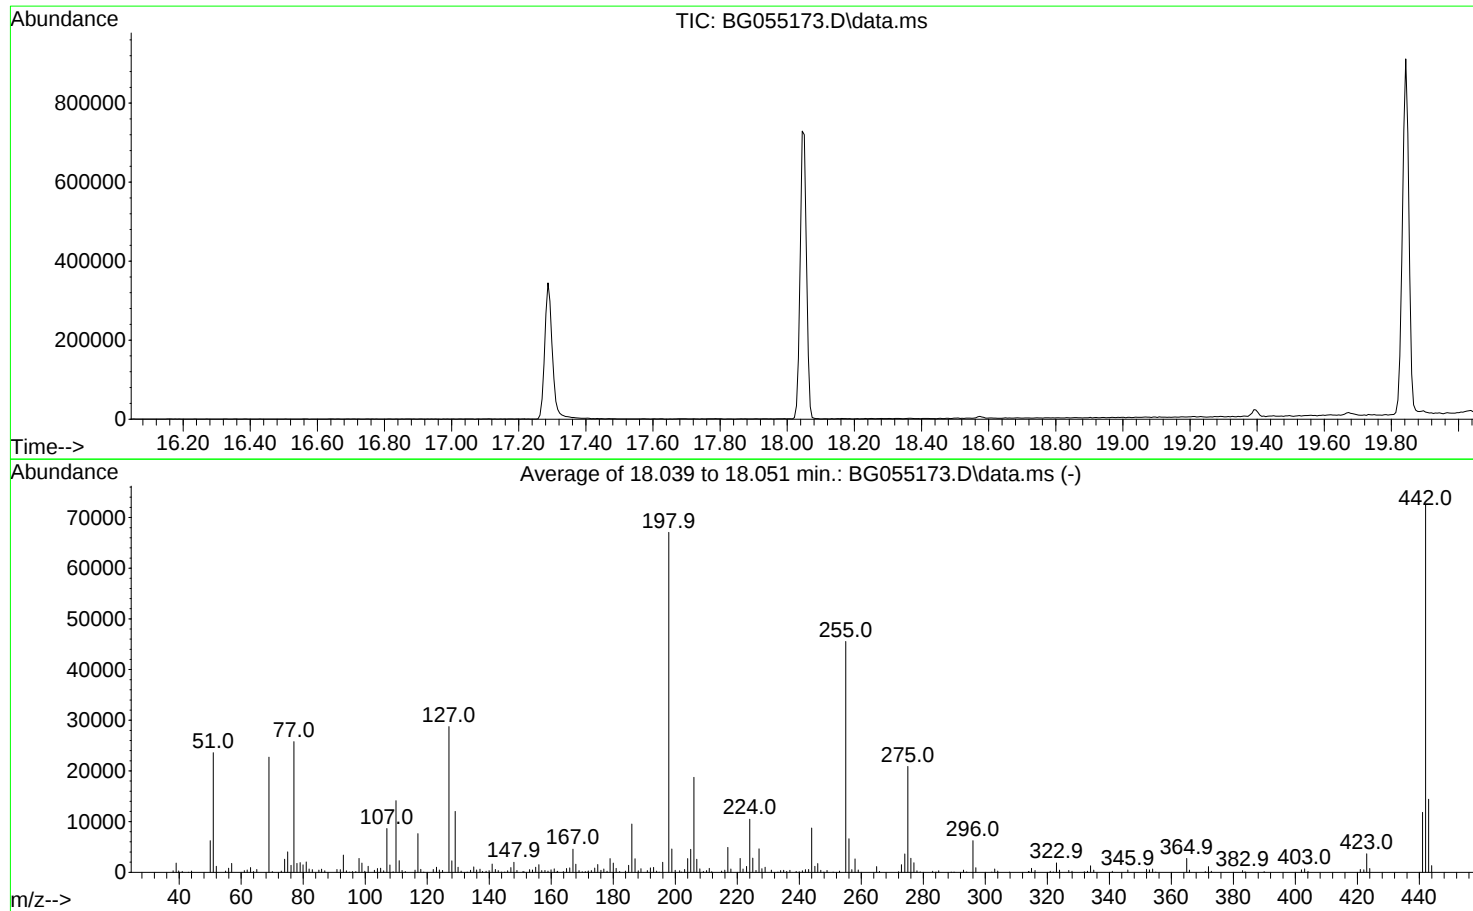




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	23584	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	22707	PASS
70	69	0.00	2	0.7	154	PASS
127	198	10	80	42.8	28733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67077	PASS
199	198	5	9	6.9	4597	PASS
275	198	10	60	31.1	20889	PASS
365	198	1	100	4.1	2736	PASS
441	198	0.01	100	17.6	11810	PASS
442	442	50	100	100.0	72579	PASS
443	442	15	24	19.9	14416	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101422\
Data File : BG055173.D
Acq On : 14 Oct 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 10:51:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

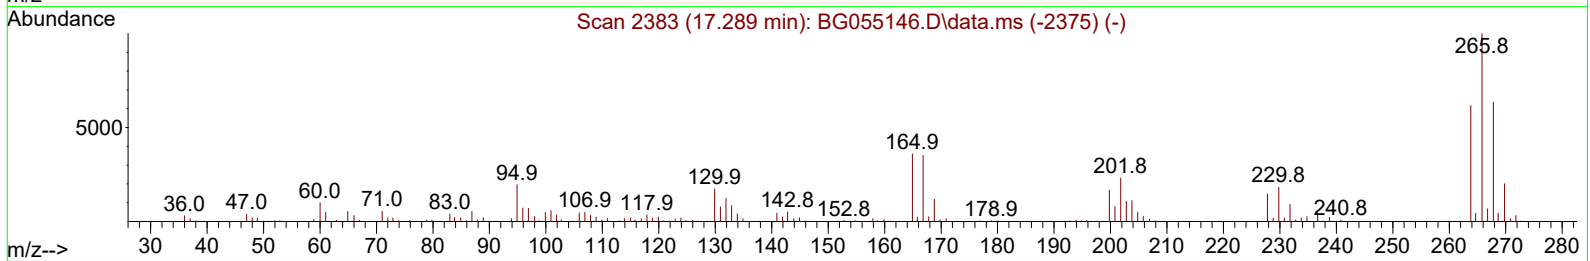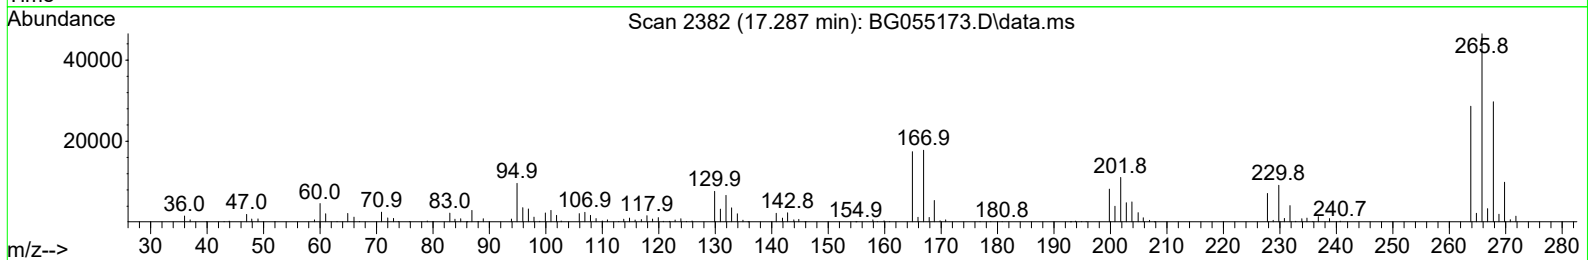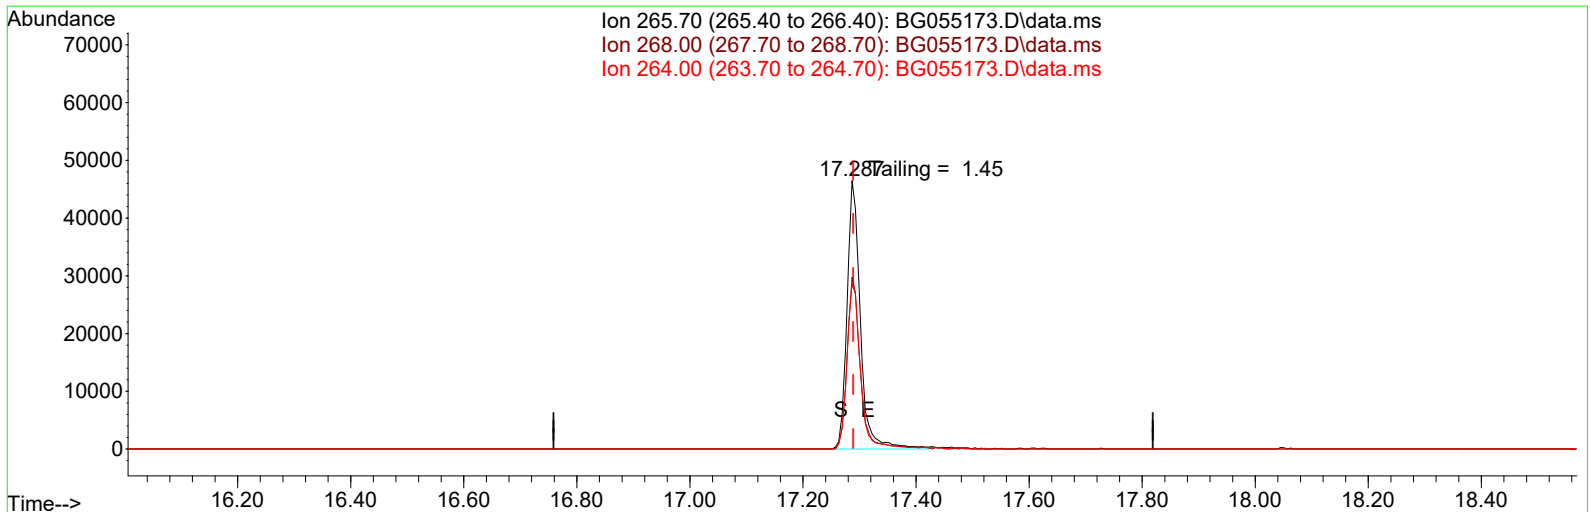

TIC: BG055173.D\data.ms

(70) Pentachlorophenol (C)

17.287min (-0.002) 26525.29 ng




response 76632

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.80	64.00
264.00	65.90	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101422\
Data File : BG055173.D
Acq On : 14 Oct 2022 10:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 14 10:51:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 05:14:13 2022
Response via : Initial Calibration

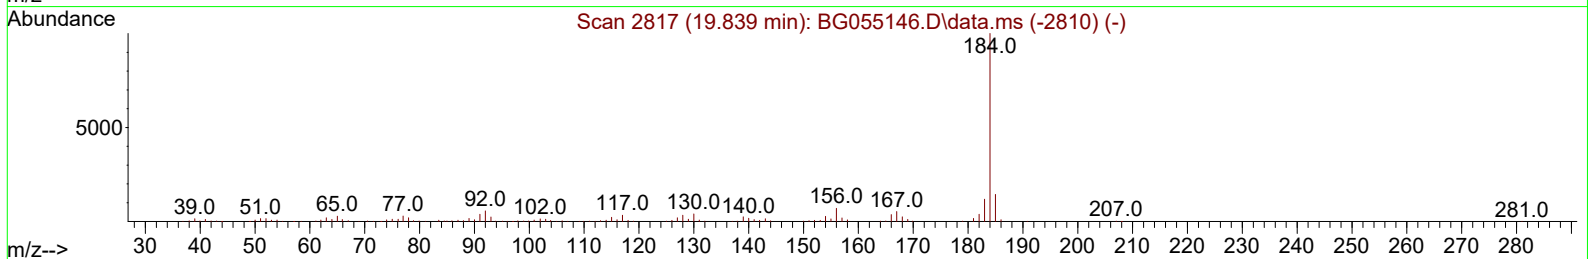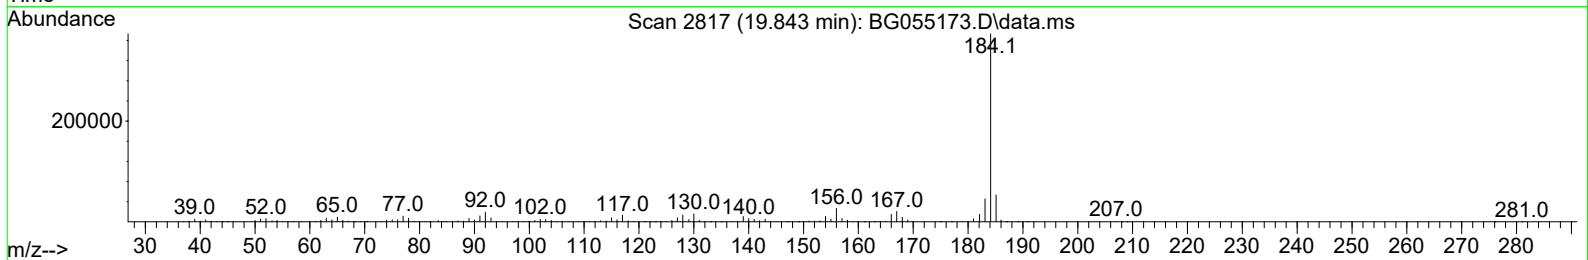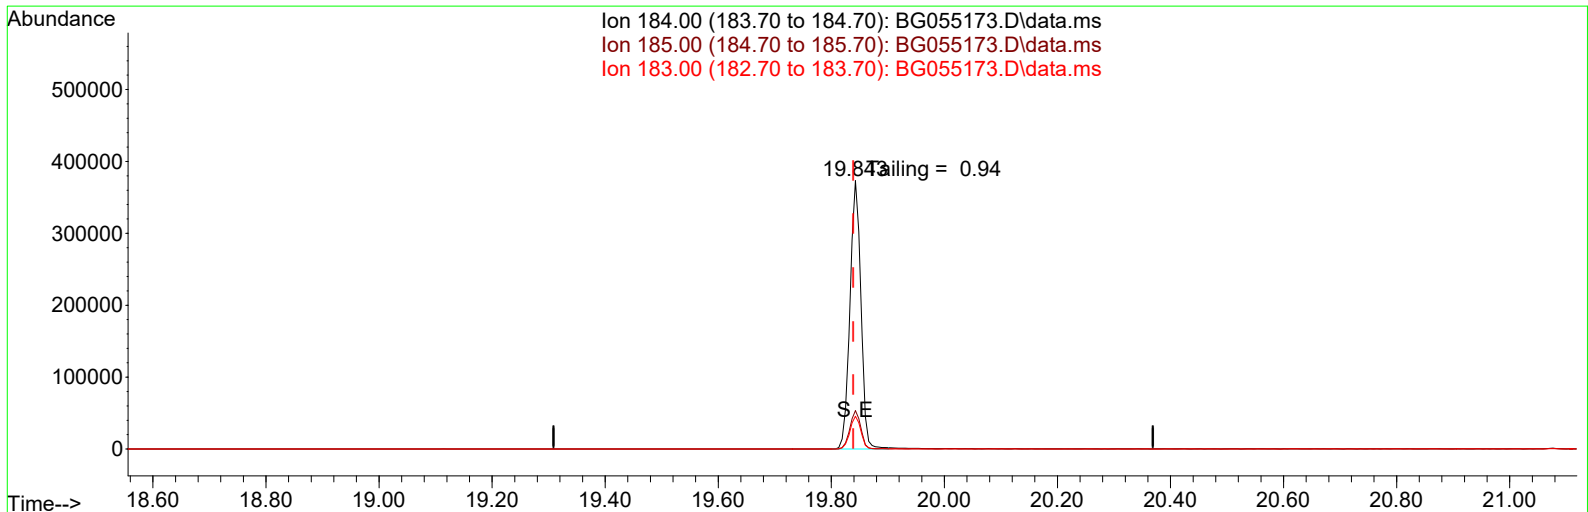

TIC: BG055173.D\data.ms

(77) Benzidine

19.843min (+ 0.004) 377093.22 ng

response 507383

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.34
183.00	11.80	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/14/2022	BNA_G	<u>BG055173.D</u>
Compound Name	Response	Retention Time
DDT	237864	21.077
DDD	5057	20.624
DDE	220	20.131
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5277	243141	2.17

Instrument :
BNA_G
ClientSampleId :
DFTPP