

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101515\
 Data File : BG019212.D
 Acq On : 15 Oct 2015 19:13
 Operator : UM/NP
 Sample : PB86110BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK10

Quant Time: Oct 16 04:08:46 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 16 04:07:16 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.00	152	13107	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	56490	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.64	164	42355	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.38	188	114257	20.00	ng/ul	0.00
78) Chrysene-d12	21.65	240	160924	20.00	ng/ul	0.00
86) Perylene-d12	24.85	264	150790	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.44	96	1601	6.80	ng/uL	0.00
5) Phenol-d5	7.17	99	35903	31.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	25693	34.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	29255	35.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.71	113	30491	31.46	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	16012	36.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	17739	38.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	31518	34.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.95	131	47213	40.07	ng/ul	0.00
44) Dimethylphthalate-d6	14.04	166	143850	38.83	ng/ul	0.00
47) Acenaphthylene-d8	14.33	160	145121	36.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	23815	35.76	ng/ul	0.00
58) Fluorene-d10	15.63	176	114206	36.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	22335	31.69	ng/ul	0.00
71) Anthracene-d10	17.48	188	206777	38.30	ng/ul	0.00
79) Pyrene-d10	19.77	212	265164	36.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.63	264	291404	38.25	ng/ul	-0.01


Target Compounds					Ovalue
15) N-Nitroso-di-n-propylamine	8.71	70	868	1.04 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101515\
Data File : BG019212.D
Acq On : 15 Oct 2015 19:13
Operator : UM/NP
Sample : PB86110BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK10

Quant Time: Oct 16 04:08:46 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 16 04:07:16 2015
Response via : Initial Calibration

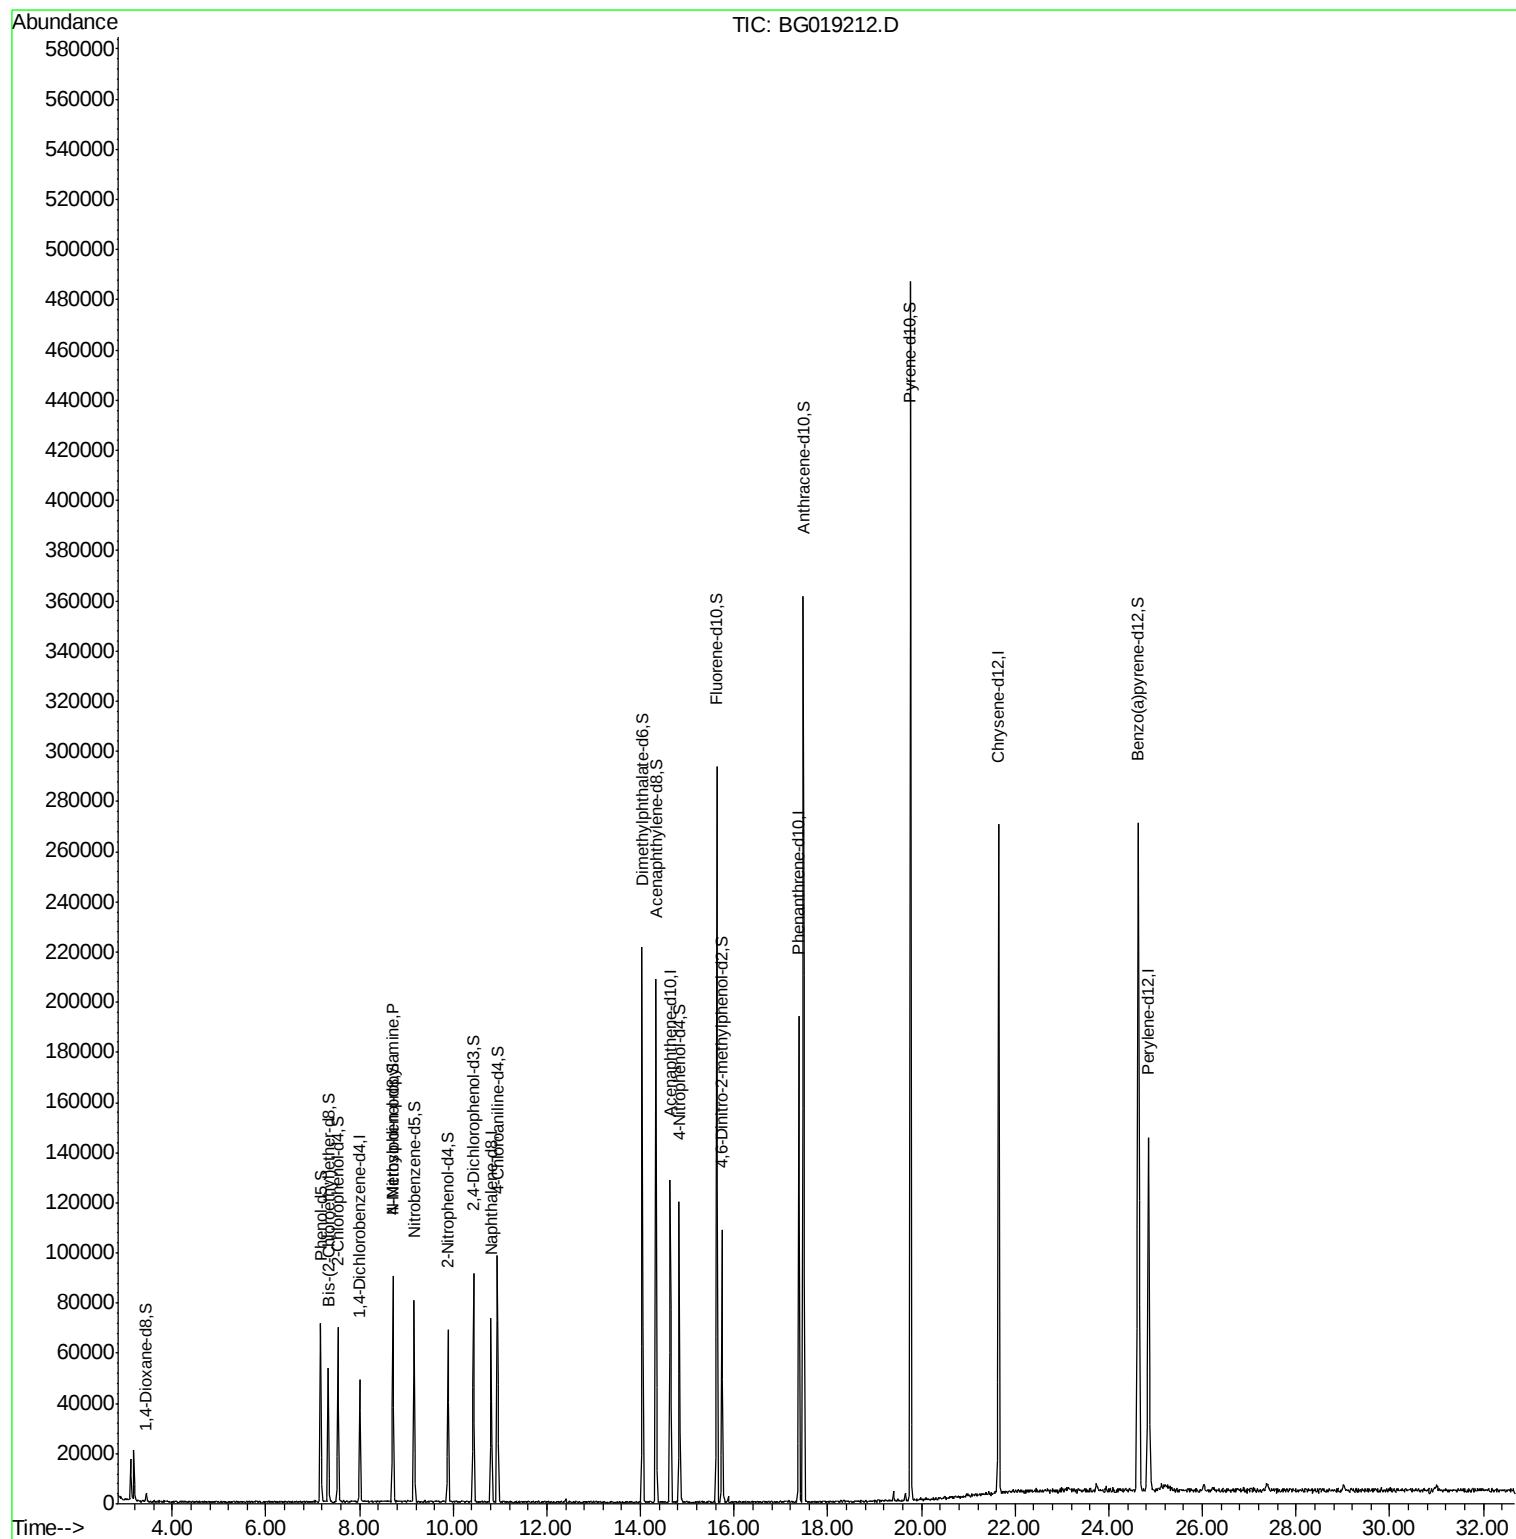

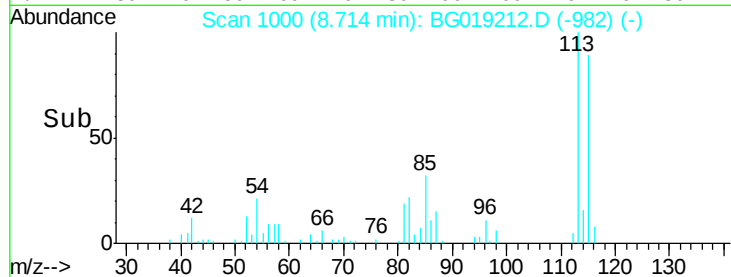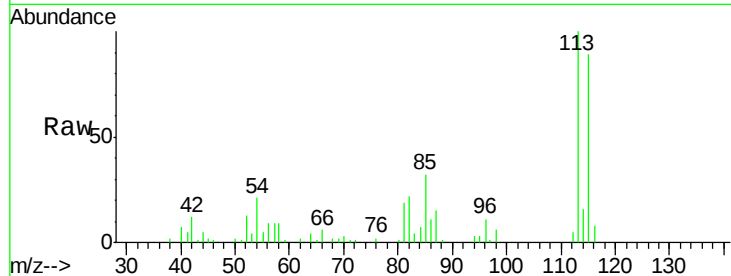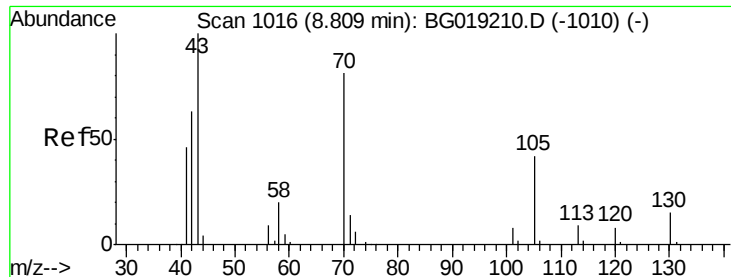

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.04 ng/ul
 RT: 8.71 min Scan# 1000
 Delta R.T. -0.10 min
 Lab File: BG019212.D
 Acq: 15 Oct 2015 19:13

Instrument :
 BNA_G
 ClientSampleId :
 SBLK10

Tot Ion: 70 Resp: 868
 Ion Ratio Lower Upper
 70 100
 42 418.1 53.6 80.4#
 101 0.0 7.9 11.9#
 130 0.0 16.5 24.7#

